Manual of Equipment register

By : SP Comnet Limited.

48/133 Soi Ramkhamhaeng 102.

High Bridge, Bangkok 10240.

Tel: 0-2373-1739.

Fax: 0-2729-3927.

Email: spcomnet@yahoo.com

website: www.medicalsoftwareonline.net

December 2012

Index

INDEX **2**

EQUIPMENT REGISTER **4**

OVERVIEW 4

EQUIPMENT REGISTER USER MANUAL 5

INSERT / UPDATE EQUIPMENT INFORMENTION **6**

INSERT / UPDATE EQUIPMENT INFORMANTION 6

ADD NEW EQUIPMENT REGISTER 6

COPY DATA 8

EDIT EQUIPMENT INFORMATION 9

EQUIPMENT SEARCH **17**

EQUIPMENT SEARCH 17

BORROW & CARRY BACK **22**

BORROW & CARRY BACK. 22

TRANSFER **25**

TRANSFER 25

MOVE LOCATION **27**

MOVE LOCATION 27

CALCULATE DEPRECIATION **29**

CALCULATE DEPRECIATION. 29

EXPORT DATA **30**

OVER VIEW 30

COST OF REPAIR 30

EQUIPMENT DATA. 31

EXPORT EQUIPMENT TEMPLATE EXCEL. 32

DISPOSE EQUIPMENT **33**

DISPOSE EQUIPMENT....33
EQUIPMENT SHOULD BE DISPOSE....33
EQUIPMENT SHOULD BE DISPOSE BY TECHNICIAN'S COMMENT....34
DISPOSED EQUIPMENT....35
PRINT LABEL....36
PRINT LABEL....36
PRINT LABEL....37
PRINT EQUIPMENT REGISTER....42
EQUIPMENT HISTORY....42

Equipment register

Overview

Equipment register is first step of working in medical equipment management system network. When purchase medical equipment to hospital by purchasing section. Equipment section will take equipment important data and issue equipment no. then record to system.

Admin group have authorize to manage about medical equipment in general like record data, change status, calculate depreciation, record distribution and print equipment register.

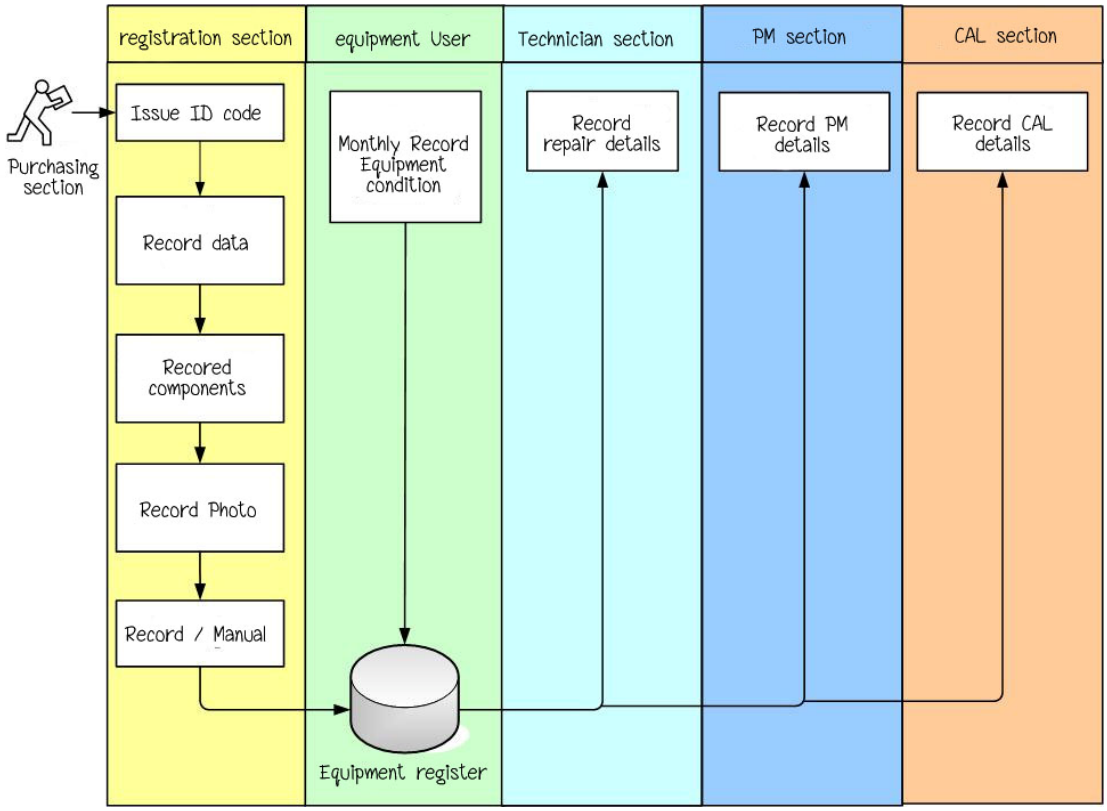

From chart after registration section record data equipment. User, Tehnician, PM, CAL section will bring recorded equipment to use. Ex :

User section can search equipment that user use for depreciation cost, repair cost, select equipment for request repair etc.

- Technician section import department data, location etc. for technician working.
- CAL and PM section specify plan for each equipment by import data into plan
  Ex: equipment user department, location, equipment category and sub-category, PM and

CAL type, PM, CAL frequency.

Equipment register user manual

Login with “Group 4 = Asset Admin”. Sub-menu follow as below.

- Insert / Update Equipment Informantion
- Epuipment Search
- Borrow & Carry Back
- Transfer
- Move Location
- Calulate Depreciation
- Export Date
- Dispose Equipment
- Print Label & Barcode
- Equipment History

Insert / Update Equipment Informention

Insert / Update Equipment Informantion

Search equipment register page for add/edit record which divided in 2 parts follow as below.

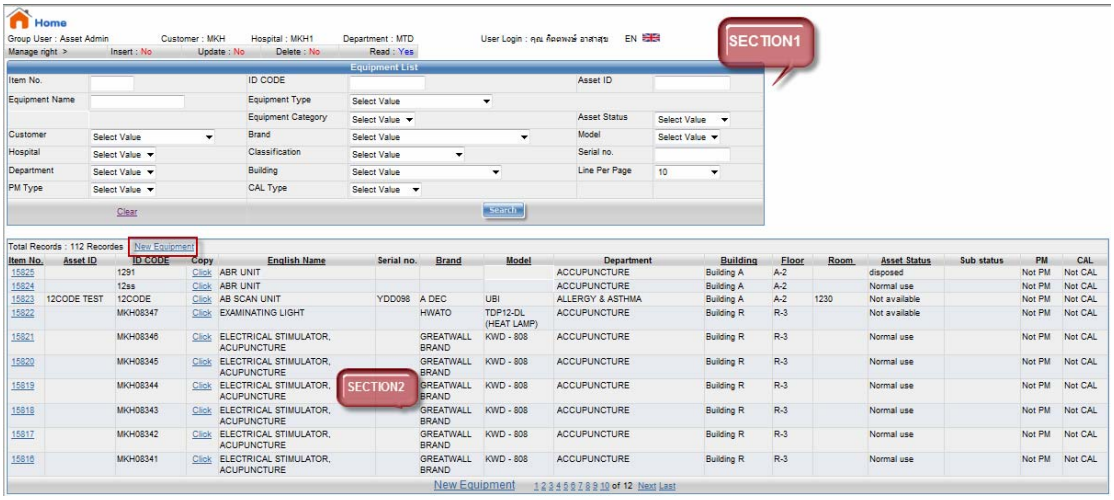

Part 1 Search area

Part 2 Show records area. In this 2 parts user able to add new record by click at “New Equipment” and edit existed record by click at record to edit.

Item No. is no. that issue for user by system which can not edit. Item no. will order by record order same as ID card no. Using equipment register in system will refer by Item No., however in real working user can specify equipment code which called ID CODE but because of in hospital network have a lot of hospitals ID CODE not allow to duplicate. Specify customer code before ID CODE is needed EX : BNH_ME 02118 .

Add new equipment register

New Equipment when click at “New Equipment” for add new equipment record, page for insert data will show up follow as below.

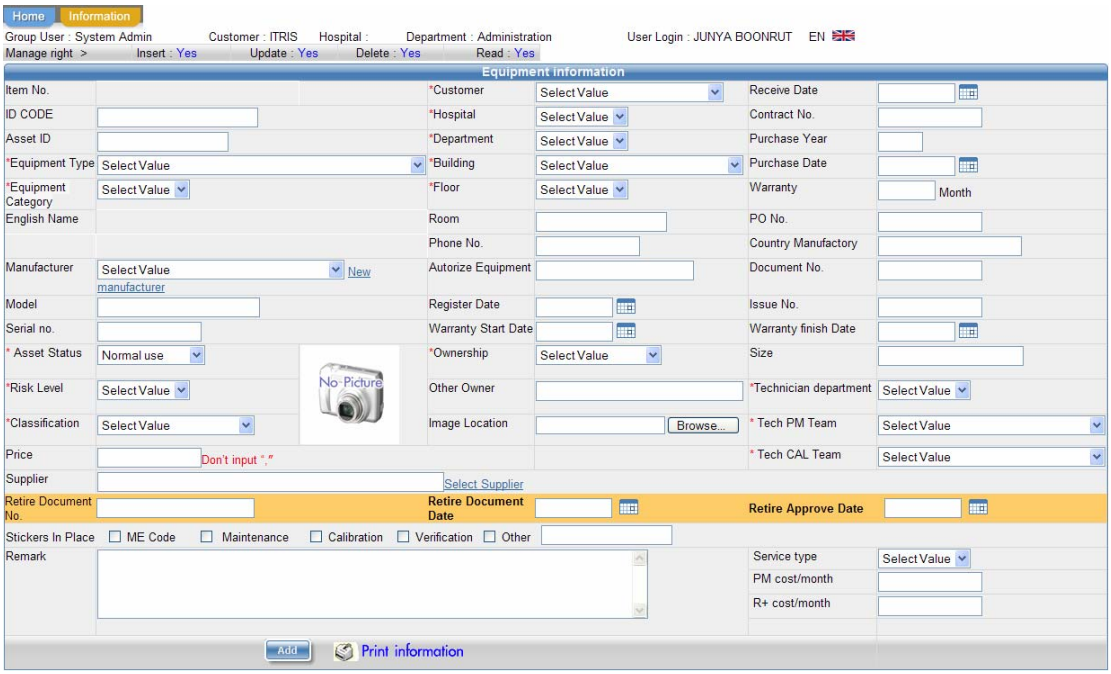

Important data need to prepare ahead for user record click to select from drop down and some data is concern as below.

Equipment category and sub-category : select category first, then select sub-categlry.

Brand and model : Select brand first, then select model.

Customer, Hospital and Department : select Customer first the, select hospital and department.

Building and floor : Select building first then select floor.

Fields with (*) required to complete field if not warning ill show up at left side on the top to warn required field, after complete all fields click “Submit” button.

Remark Fields with (*) is required is user not complete required fields when click “Add” button warning will show up.

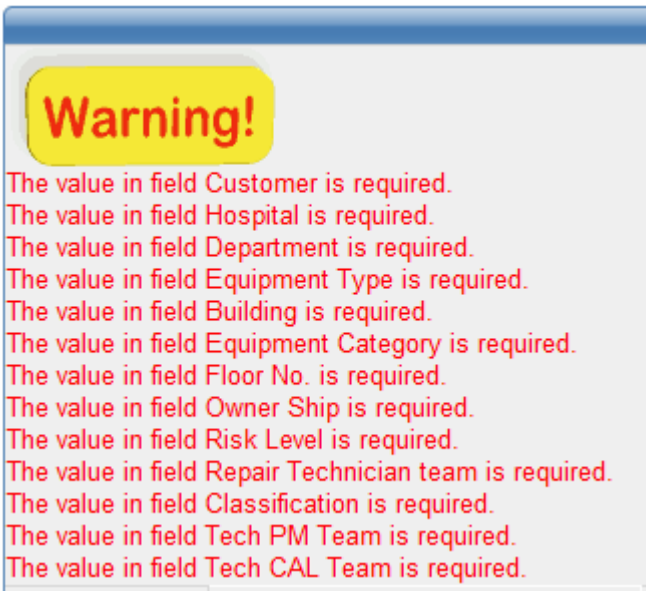
Warning!
The value in field Customer is required.
The value in field Hospital is required.
The value in field Department is required.
The value in field Equipment Type is required.
The value in field Building is required.
The value in field Equipment Category is required.
The value in field Floor No. is required.
The value in field Owner Ship is required.
The value in field Risk Level is required.
The value in field Repair Technician team is required.
The value in field Classification is required.
The value in field Tech PM Team is required.
The value in field Tech CAL Team is required.

Copy data

Copy data is adding new equipment register by copy exist equipment record which have same data for save time and not insert all details. Using method.

- Click in copy column of record needed to copy.

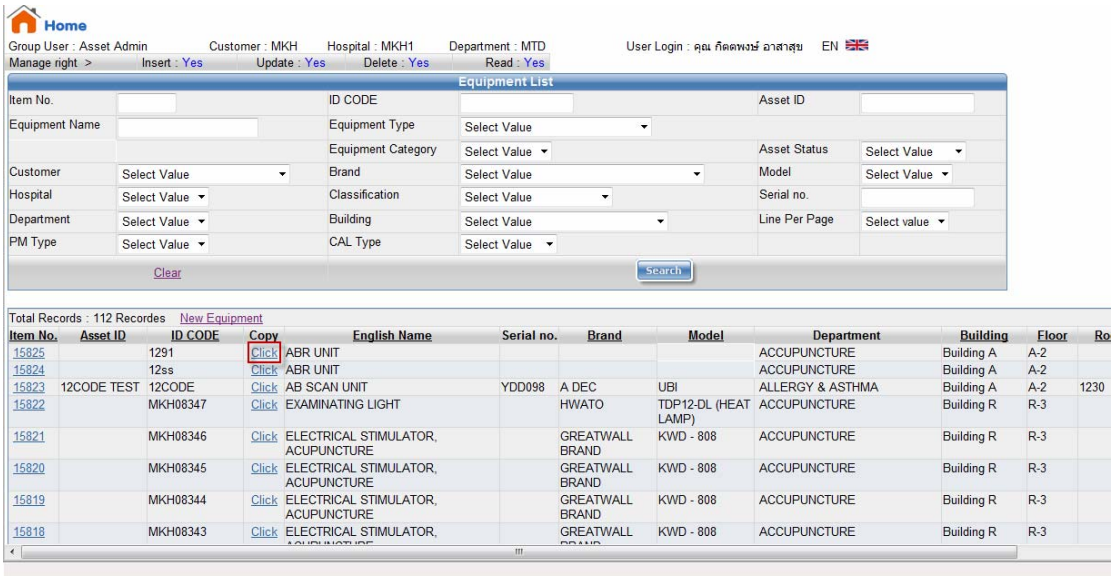
Home
Group User : Asset Admin
Customer : MKH
Hospital : MKH1
Department : MTD
User Login : คุณ กิตตพงษ์ อาสาสุข
EN
Manage right > Insert : Yes Update : Yes Delete : Yes Read : Yes
Equipment List
Item No.
ID CODE
Asset ID
Equipment Name
Equipment Type
Select Value
Equipment Category
Asset Status
Customer
Brand
Model
Hospital
Classification
Serial no.
Department
Building
Line Per Page
PM Type
CAL Type
Clear
Search
Total Records : 112 Recordes
New Equipment
Item No. | Asset ID | ID CODE | Copy | English Name | Serial no. | Brand | Model | Department | Building | Floor | Ro
15825 | | 1291 | Click | ABR UNIT | | | | ACCUPUNCTURE | Building A | A-2 |
15824 | | 12ss | Click | ABR UNIT | | | | ACCUPUNCTURE | Building A | A-2 |
15823 | 12CODE TEST | 12CODE | Click | AB SCAN UNIT | YDD098 | A DEC | UBI | ALLERGY & ASTHMA | Building A | A-2 | 1230
15822 | | MKH08347 | Click | EXAMINATING LIGHT | | HWATO | TDP12-DL (HEAT LAMP) | ACCUPUNCTURE | Building R | R-3 |
15821 | | MKH08346 | Click | ELECTRICAL STIMULATOR, ACUPUNCTURE | | GREATWALL BRAND | KWD - 808 | ACCUPUNCTURE | Building R | R-3 |
15820 | | MKH08345 | Click | ELECTRICAL STIMULATOR, ACUPUNCTURE | | GREATWALL BRAND | KWD - 808 | ACCUPUNCTURE | Building R | R-3 |
15819 | | MKH08344 | Click | ELECTRICAL STIMULATOR, ACUPUNCTURE | | GREATWALL BRAND | KWD - 808 | ACCUPUNCTURE | Building R | R-3 |
15818 | | MKH08343 | Click | ELECTRICAL STIMULATOR, | | GREATWALL | KWD - 808 | ACCUPUNCTURE | Building R | R-3 |

- Page for enter new equipment record's ID CODE no. will show up and show copy from which old ID CODE when sure to copy click "Comfirm copy". If want to copy new record <with same old copied ID CODE> enter new ID CODE and Confirm copy until finish.

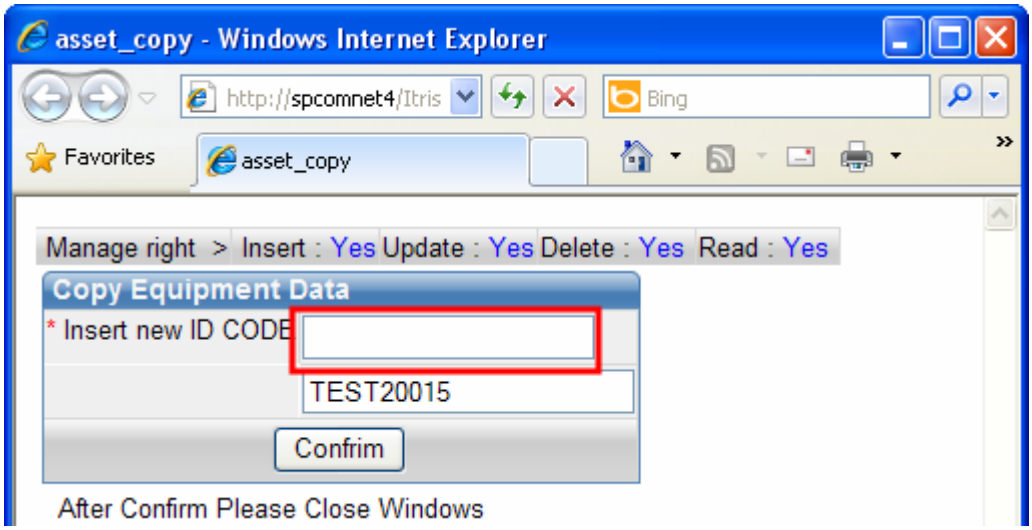

- To cancel click X (Cross) on the top right for close page.

Edit equipment information

Edit existed equipment information click at "Item No." to edit, divided in 9 pages follow as below.

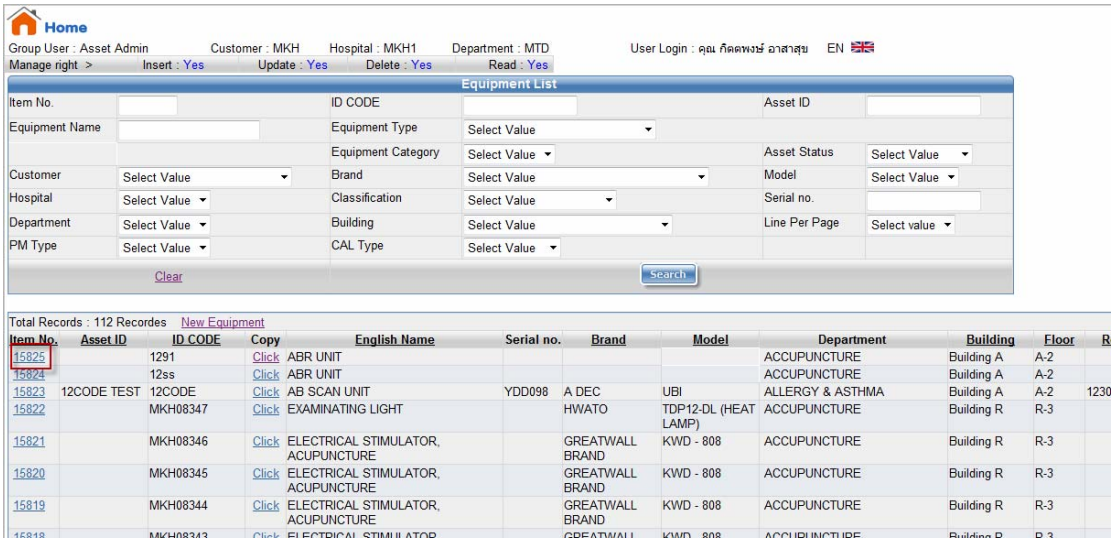
Home
Group User : Asset Admin
Customer : MKH
Hospital : MKH1
Department : MTD
User Login : คุณ กิตตพงษ์ อาสาสุข
EN
Manage right > Insert : Yes Update : Yes Delete : Yes Read : Yes
Equipment List
Item No.
ID CODE
Asset ID
Equipment Name
Equipment Type
Select Value
Equipment Category
Asset Status
Customer
Brand
Model
Hospital
Classification
Serial no.
Department
Building
Line Per Page
PM Type
CAL Type
Clear
Search
Total Records : 112 Recordes
New Equipment
Item No. Asset ID ID CODE Copy English Name Serial no. Brand Model Department Building Floor
15825 1291 Click ABR UNIT ACCUPUNCTURE Building A A-2
15824 12ss Click ABR UNIT ACCUPUNCTURE Building A A-2
15823 12CODE TEST 12CODE Click AB SCAN UNIT YDD098 A DEC UBI ALLERGY & ASTHMA Building A A-2
15822 MKH08347 Click EXAMINATING LIGHT HWATO TDP12-DL (HEAT LAMP) ACCUPUNCTURE Building R R-3
15821 MKH08346 Click ELECTRICAL STIMULATOR, ACUPUNCTURE GREATWALL BRAND KWD - 808 ACCUPUNCTURE Building R R-3
15820 MKH08345 Click ELECTRICAL STIMULATOR, ACUPUNCTURE GREATWALL BRAND KWD - 808 ACCUPUNCTURE Building R R-3
15819 MKH08344 Click ELECTRICAL STIMULATOR, ACUPUNCTURE GREATWALL BRAND KWD - 808 ACCUPUNCTURE Building R R-3

- Equipment information, this page same as New Equipment page.

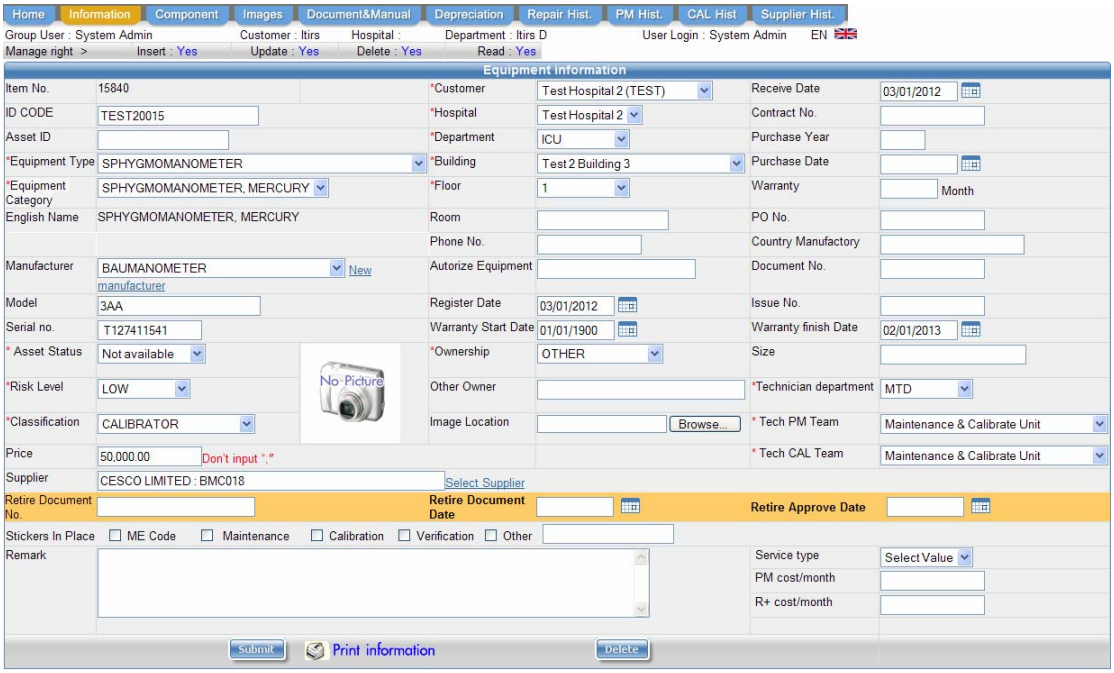

- Add equipment photo : only 1 image for each equipment.

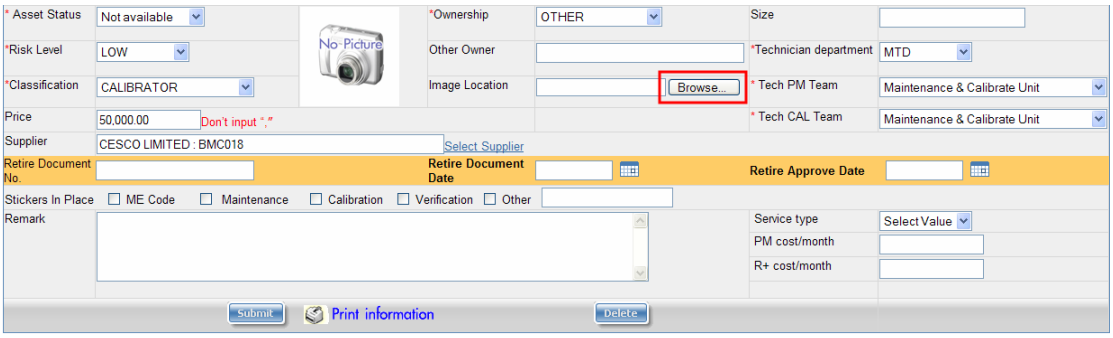

- To add photo click Browse, pop up for select photo in personal PC or in Flash drive will show up. User shoul re-size photo to 100 pixcels.

- Select photo and click “Open” button.

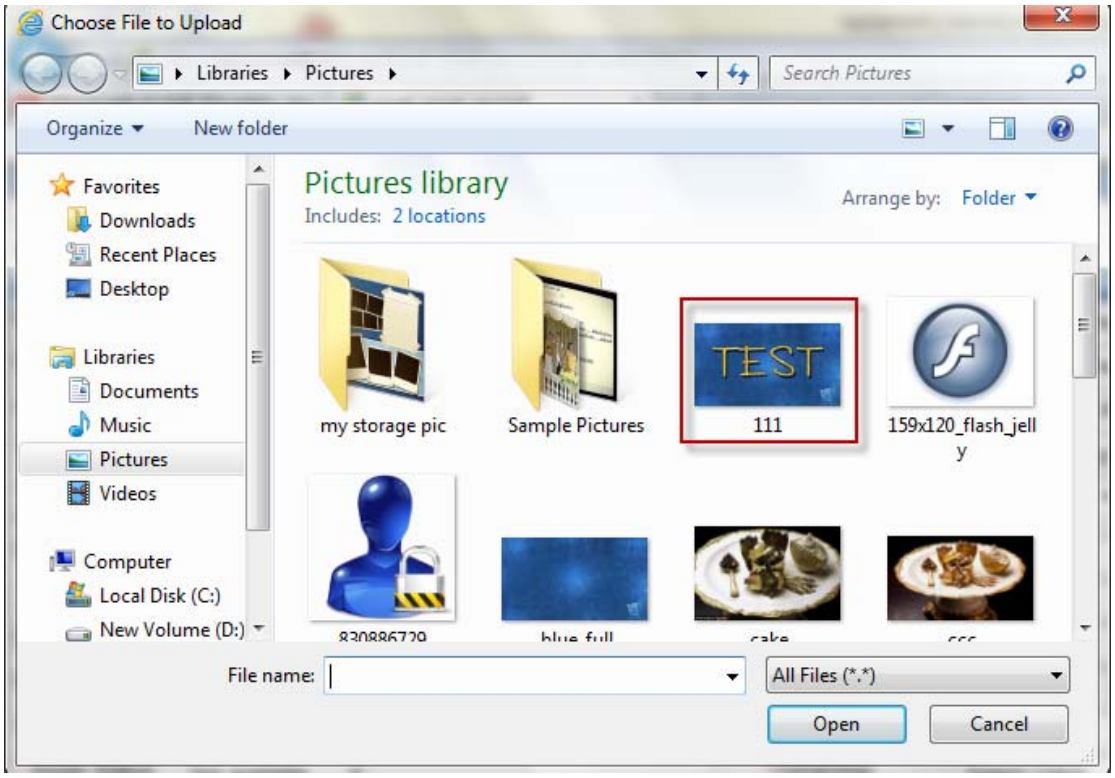

- Selected photo will show at page, click Submit button to save photo in database.

- Print information, click Print information.

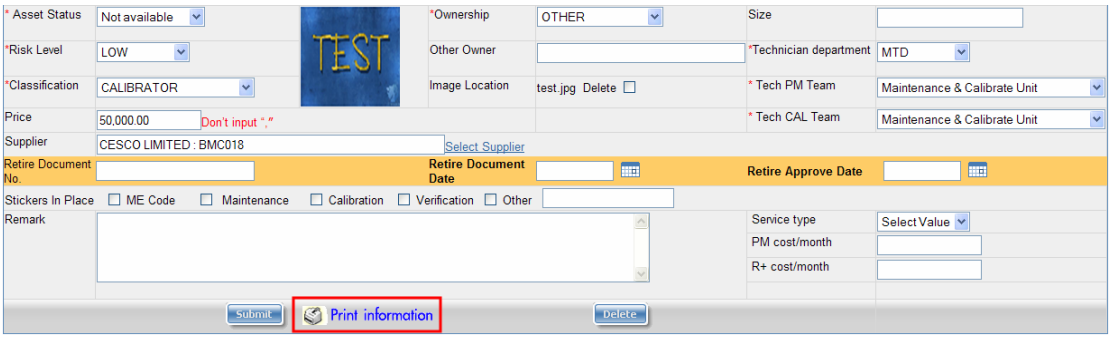

Equipment register will appear.

- Component is equipment component record page (option).

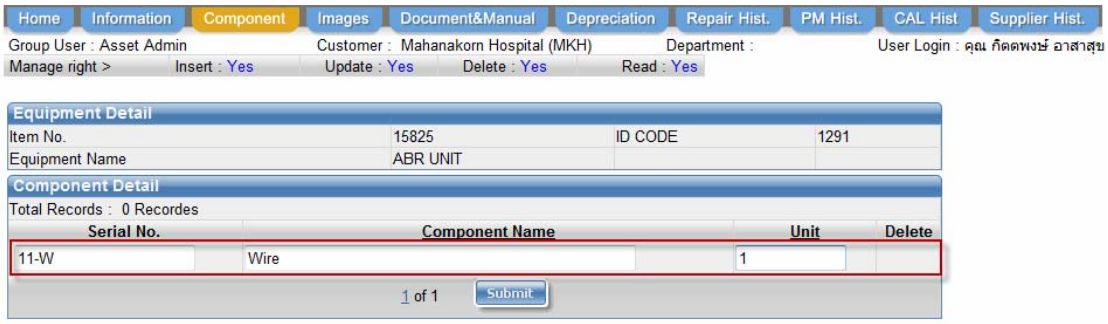

Enter code, name and quantity. After click Submit button new line will appear at the bottom of record for insert next record.

- Images for record equipment photo other than main photo. User also record component, location and person who responsible with unlimited quantity.

Add photo : follow as below.

1. Add photo Click at Add/Edit Images.

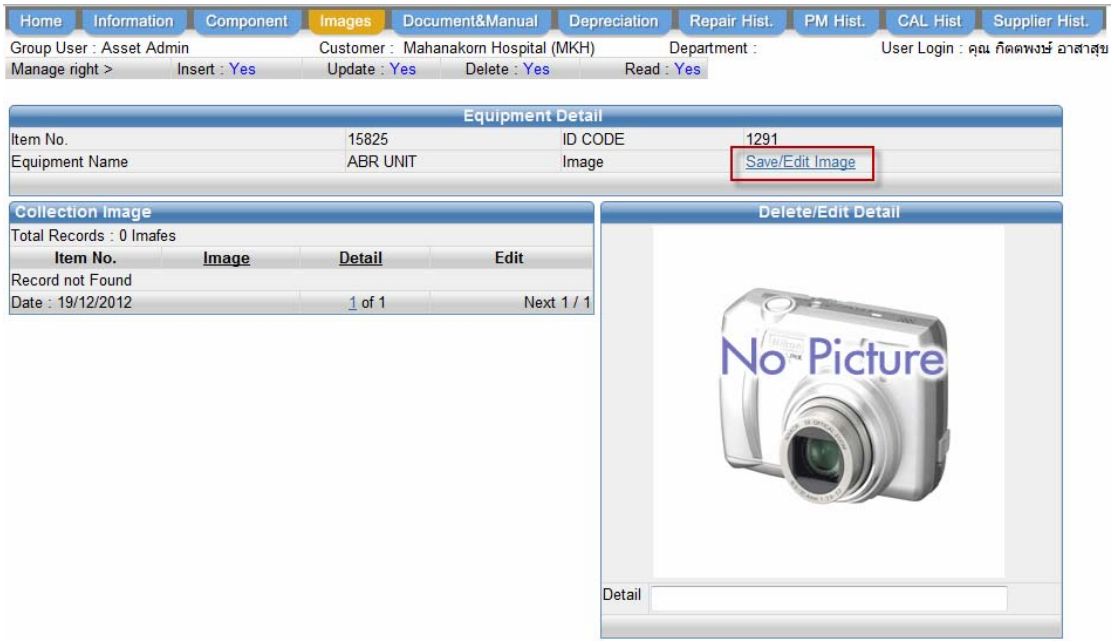

2. Click Insert Images to ad new photo.

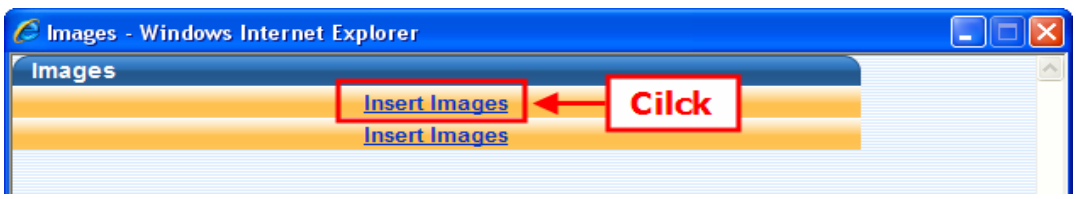

3. User can add 10 photo per time, insert details and click Browse for select photo.

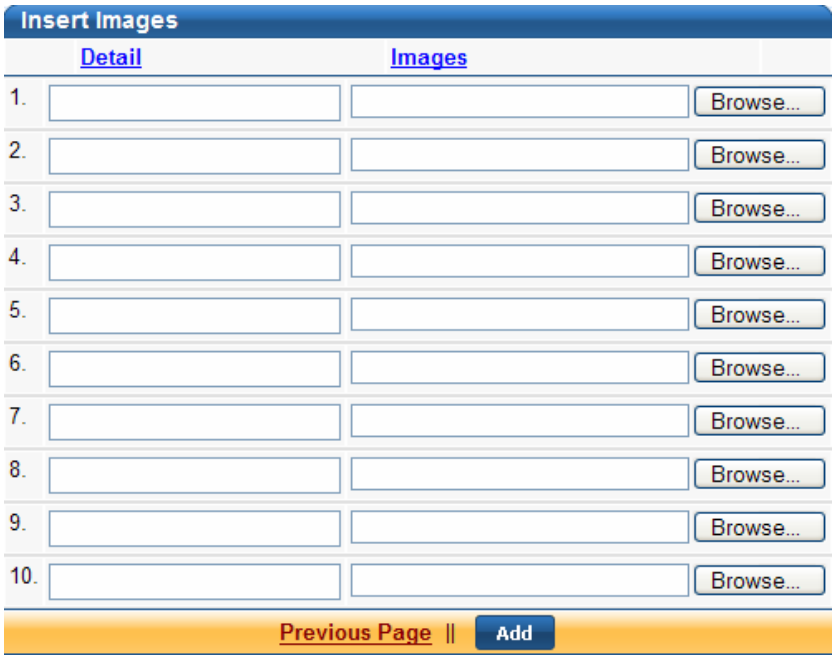

After done click “Add” button.

- Dcoument and Manual, In this day sending Equipment manual as PDF file is famous user able to attach PDF, Word ,Excel , Power point file etc….. with equipment details

1. Insert No. and click Browse for select document.

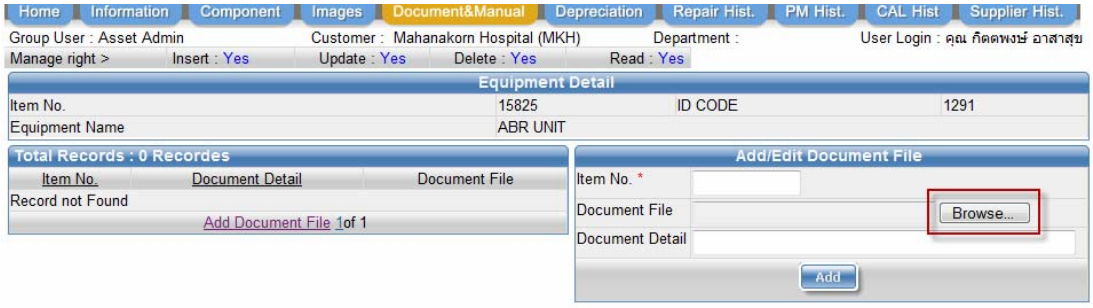

2. Select document to attach and click Open.

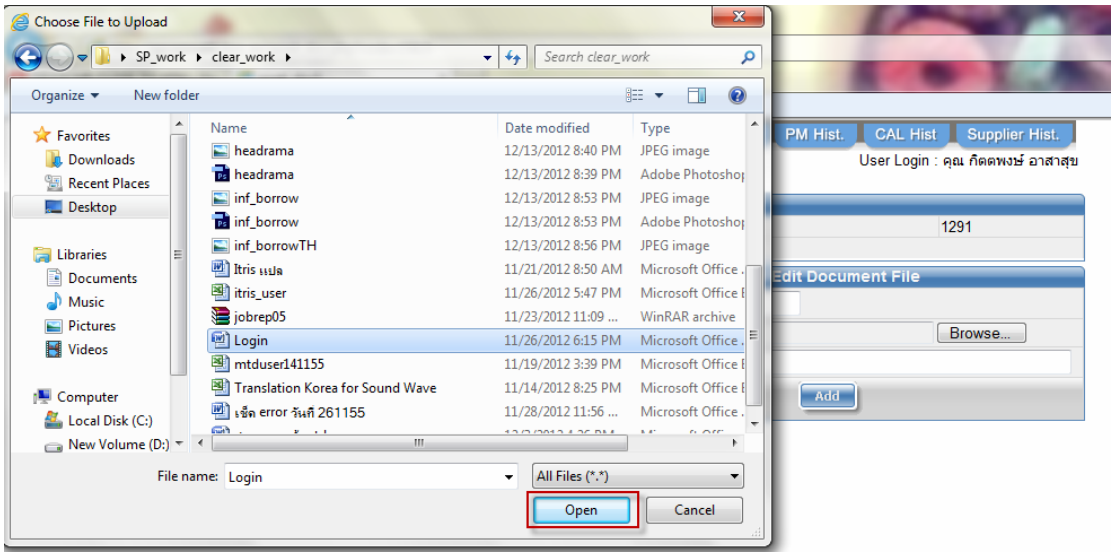

3. Insert document details and click “Add” button for record.

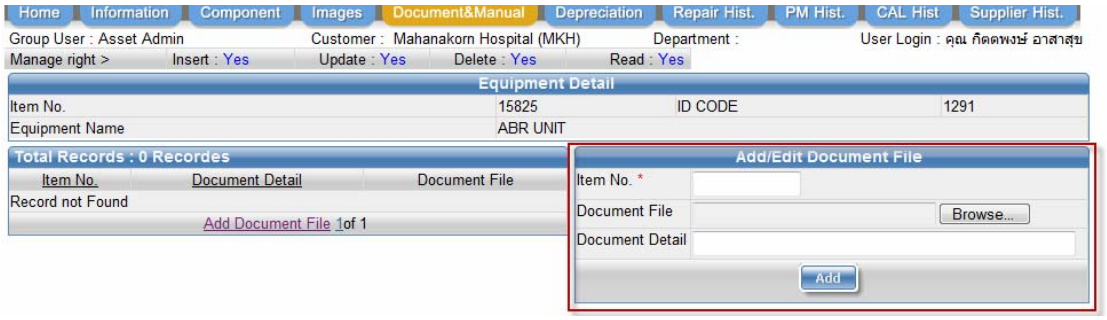

4. To edit.

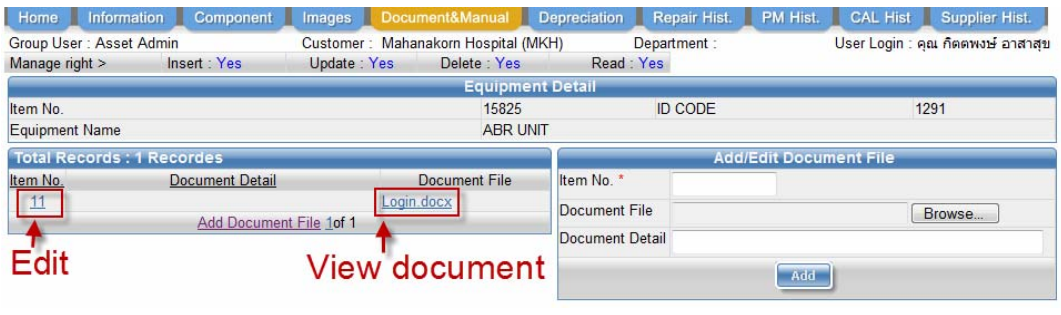

- Depreciation divided in 2 parts : record part is on the left side. Depreciation data should be consist by :
  - Calculcate depreciation start date.
  - Purchase price.
  - Quantity of useful year.
  - Scrap value

  Required to insert details for all equipment and PM in the end of every month. In Depreciation process menu process result will appear on the right side consist by Calculate depreciation year and month.

- Monthly depreciation.

- Yearly depreciation.
- Accumulate depreciation.
- Book Value.

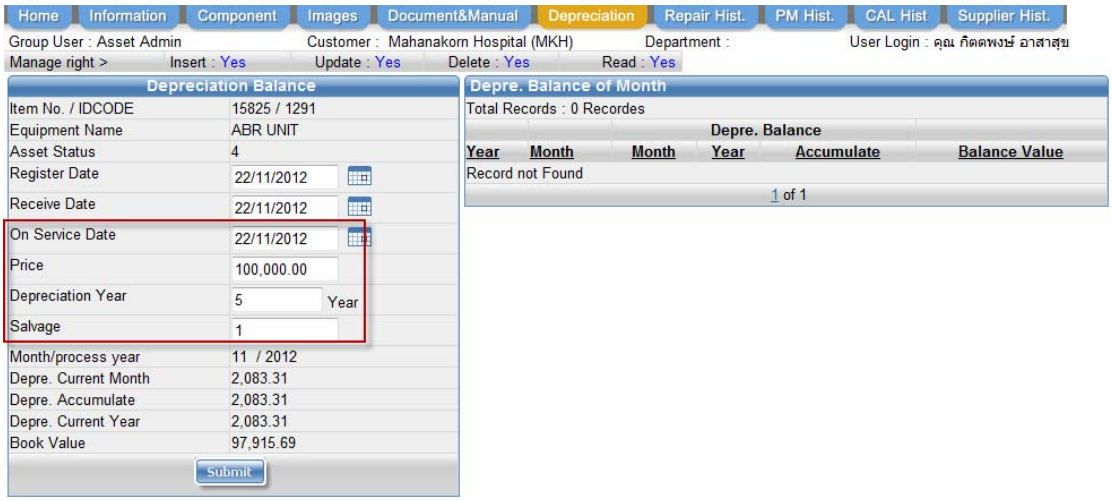

- Repair hist. for view repair history that how many times of repair. Repair history page data import from working result of technician section.

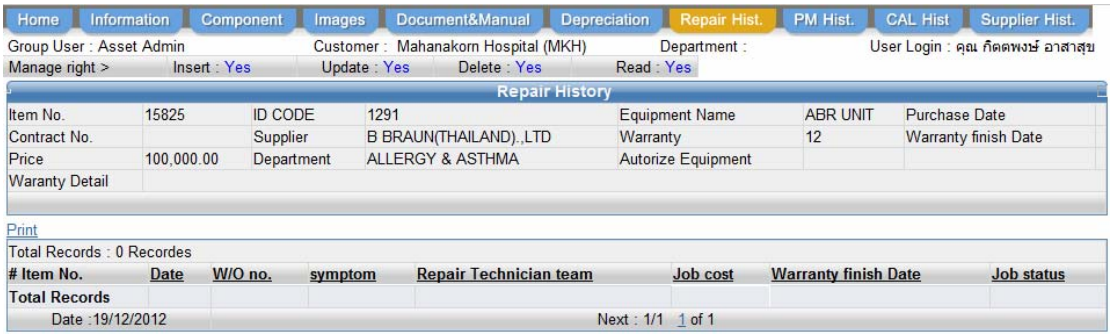

User can click to view details of each time by clic at repair order no. which user want to view.

- PM hist. for view PM history which how much this equipment pass PM. PM history data import from working result of PM section.

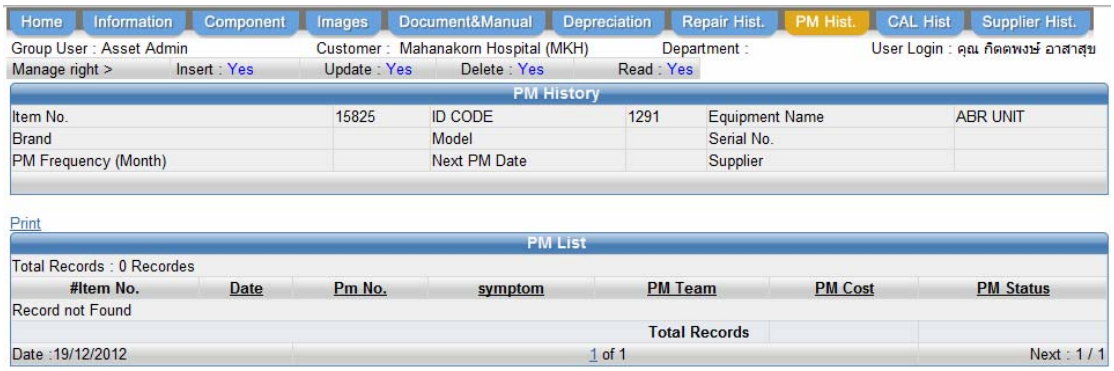

User can click to view PM details by click at PM order no.

- CAL hist. for view CAL history which how much this equipment pass CAL. CAL history data import from working result of CAL section.

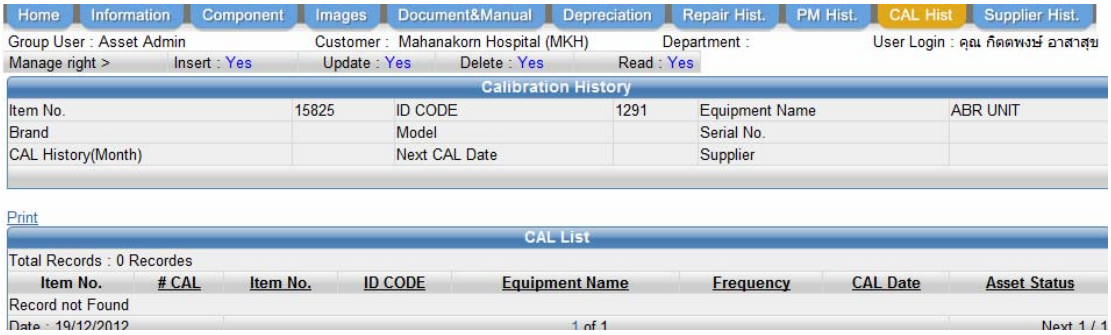

User can click to view CAL details by click at CAL order no.

- Supplier hist. data import from Send to outsource record.

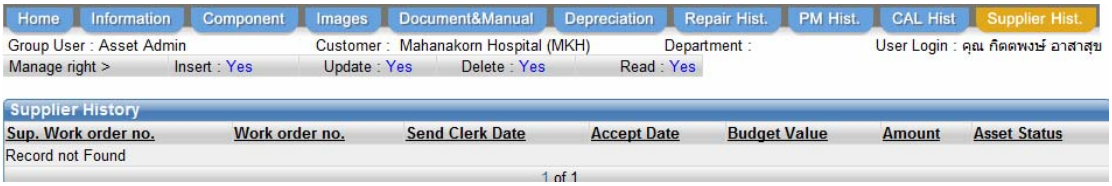

Equipment Search

Equipment Search

Equipment search for search and view equipment details only can not edit records.

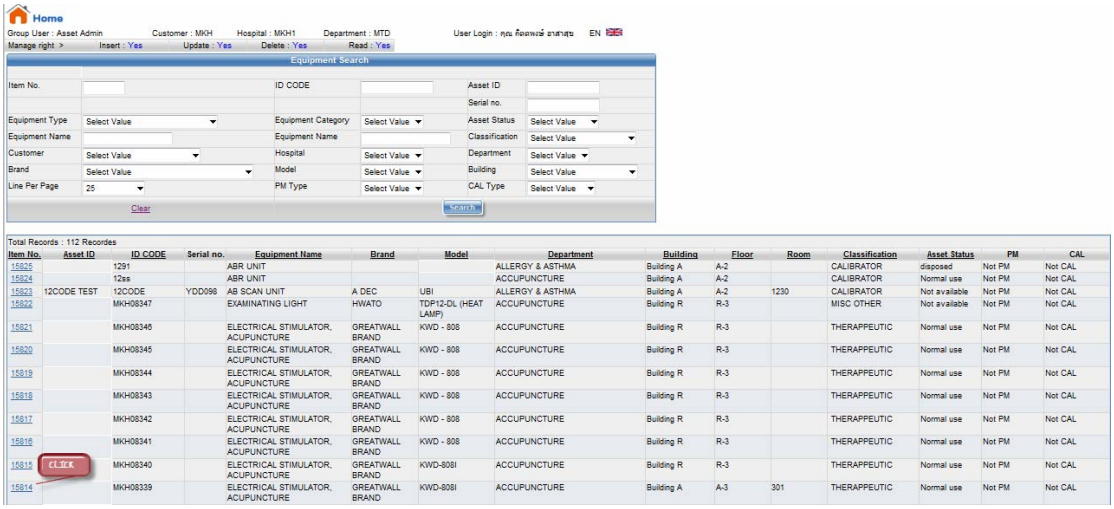

User can select equipment by clikc in “Item No.” column. After click will enter to View details page and click at menu on the left side to view.

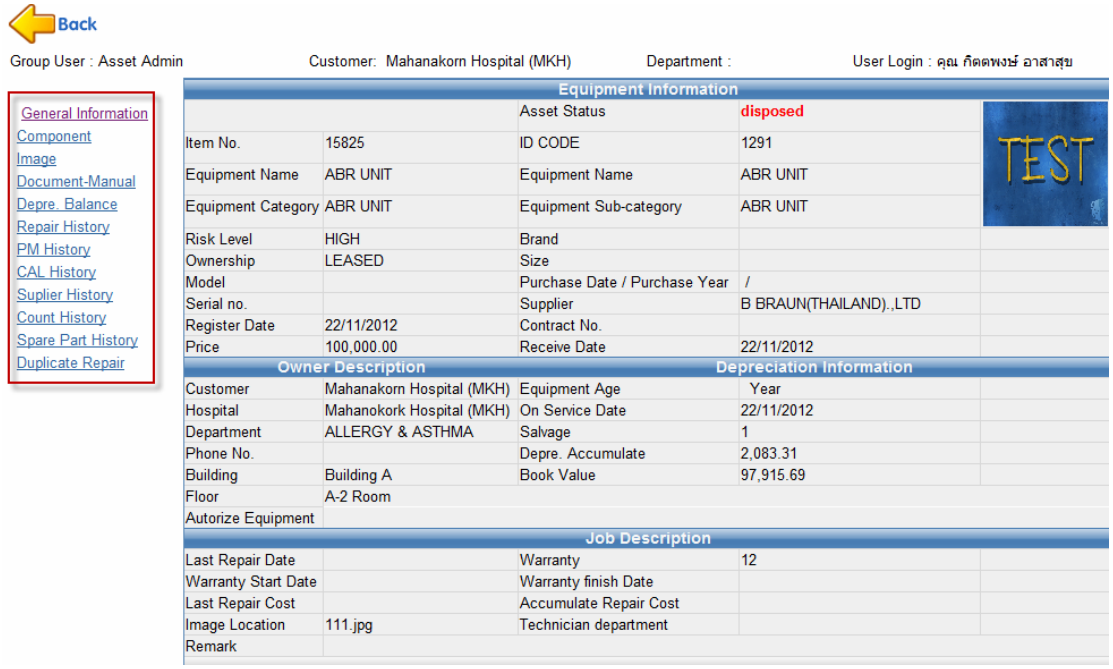

- Component.

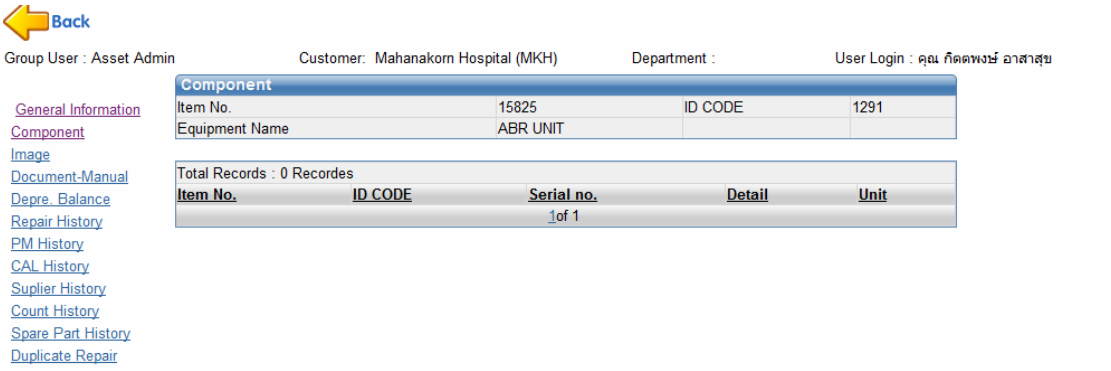

- Image

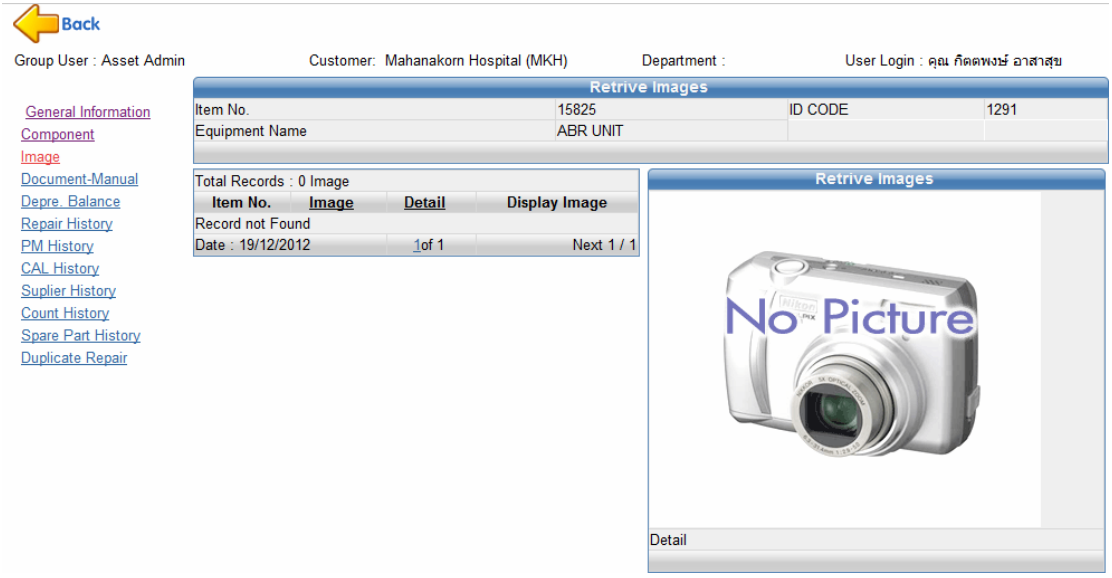

Click in “Display Image” column to view large size of photo.

- Document-Manual.

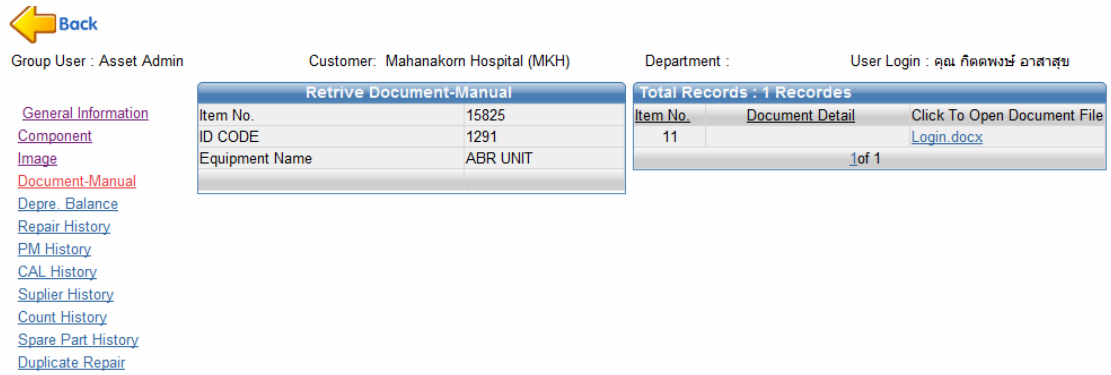

Able to view document by click open document file.

- Depreciation.

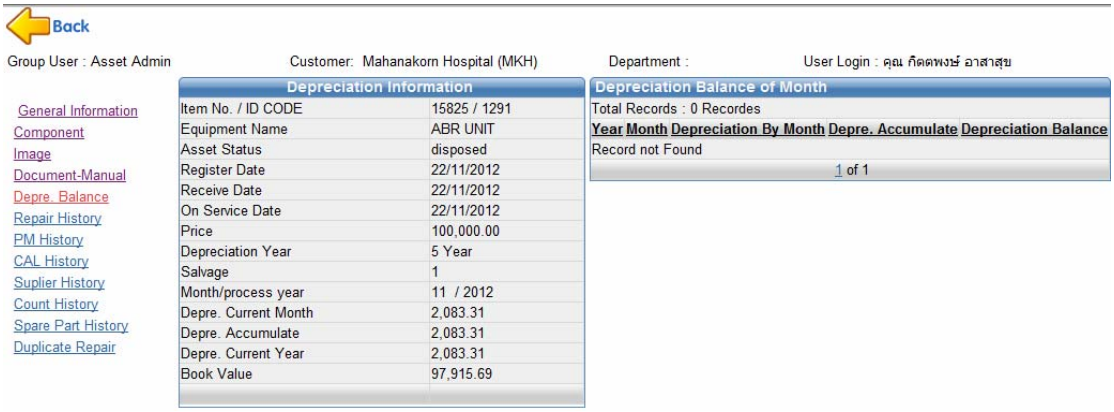

- Repair history.

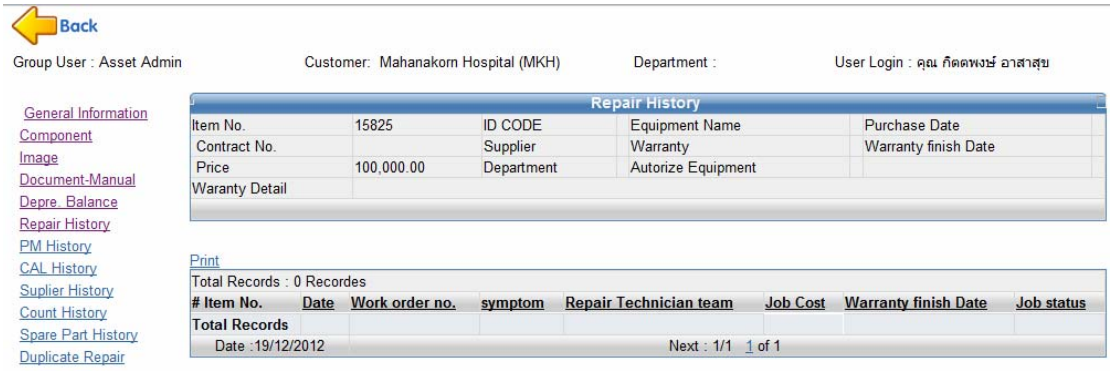

Click at Repair order no. to view repair details.

- PM history.

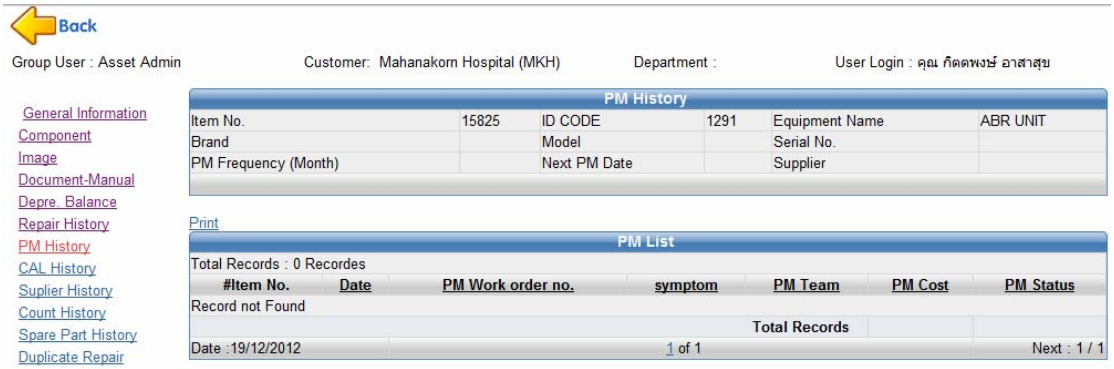

- CAL history.

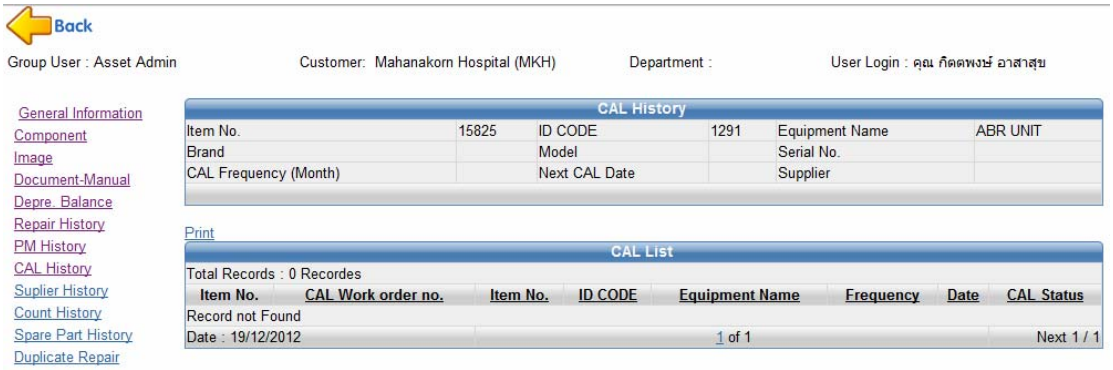

- Supplier history.

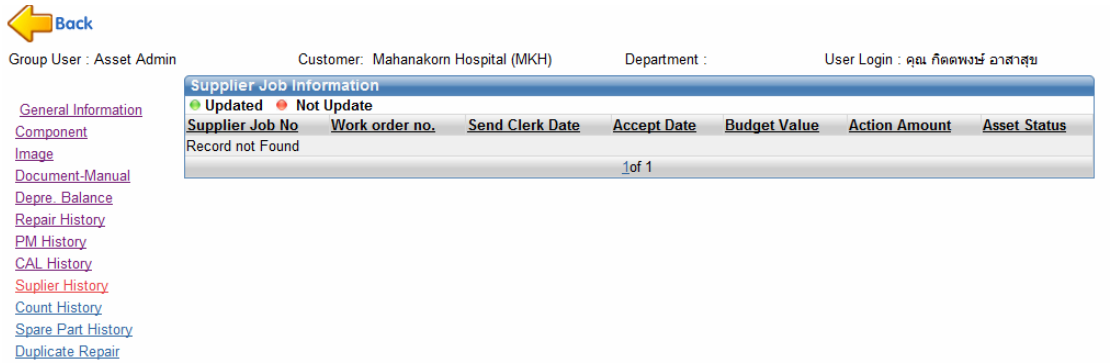

- Count history.

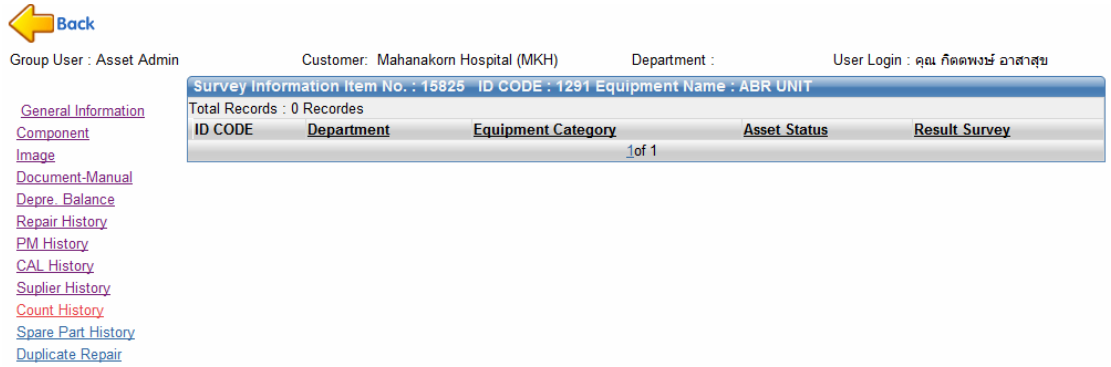

- Spare parts history.

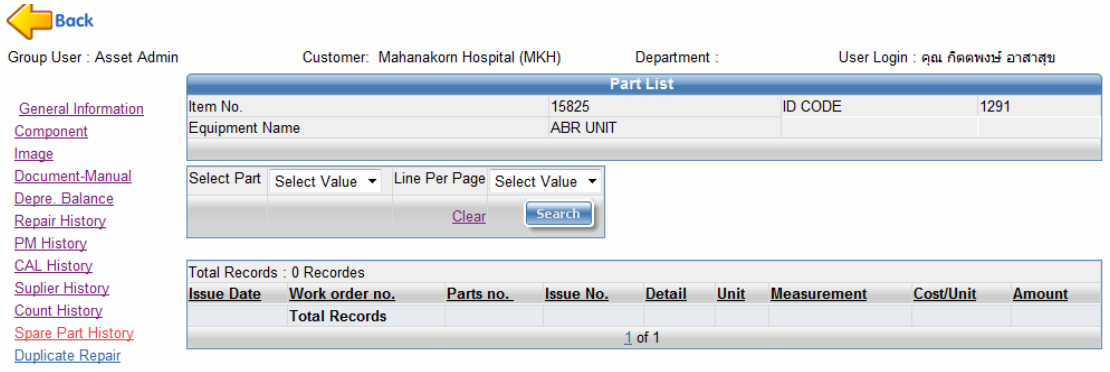

- Duplicate repair.

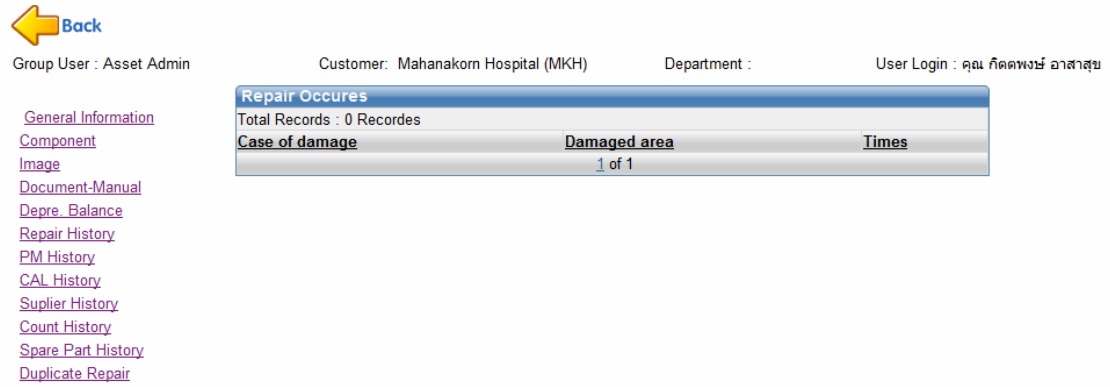

Borrow & Carry Back

Borrow & Carry Back.

For owner department record equipment borrow-return details for record history. In borrow and return also process in process in monthly examine equipment. If borrow without record, user need to record details into Borrow-Return system.

Borrow equipment should be equipment not in during repair and not medical center equipment.

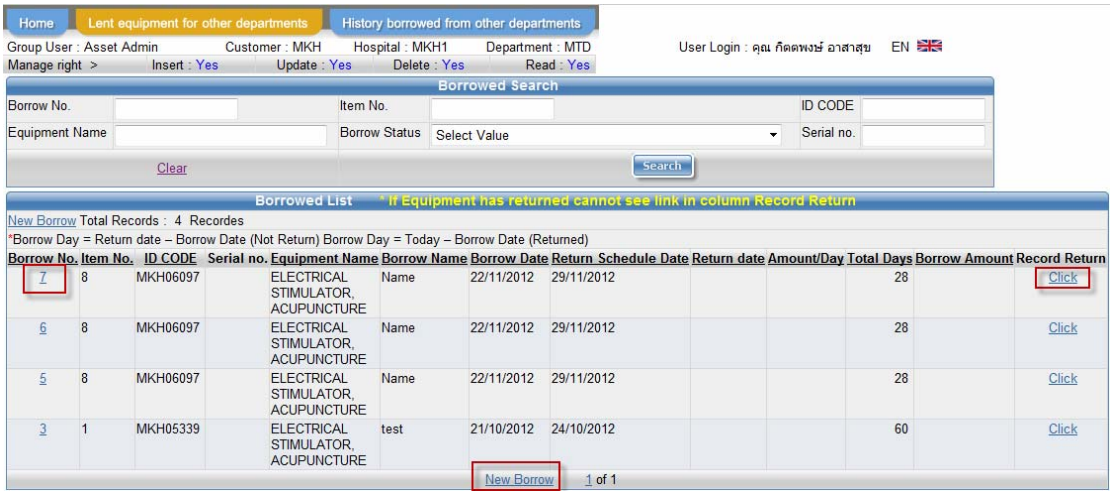
Home
Lent equipment for other departments
History borrowed from other departments
Group User : Asset Admin
Customer : MKH
Hospital : MKH1
Department : MTD
User Login : คุณ กิตพงษ์ อาสาสุข
EN
Manage right >
Insert : Yes
Update : Yes
Delete : Yes
Read : Yes
Borrowed Search
Borrow No.
Item No.
ID CODE
Equipment Name
Borrow Status
Select Value
Serial no.
Clear
Search
Borrowed List
* If Equipment has returned cannot see link in column Record Return
New Borrow Total Records : 4 Recordes
*Borrow Day = Return date – Borrow Date (Not Return) Borrow Day = Today – Borrow Date (Returned)
Borrow No. | Item No. | ID CODE | Serial no. | Equipment Name | Borrow Name | Borrow Date | Return Schedule Date | Return date | Amount/Day | Total Days | Borrow Amount | Record Return
7 | 8 | MKH06097 | | ELECTRICAL STIMULATOR, ACUPUNCTURE | Name | 22/11/2012 | 29/11/2012 | | | 28 | | Click
6 | 8 | MKH06097 | | ELECTRICAL STIMULATOR, ACUPUNCTURE | Name | 22/11/2012 | 29/11/2012 | | | 28 | | Click
5 | 8 | MKH06097 | | ELECTRICAL STIMULATOR, ACUPUNCTURE | Name | 22/11/2012 | 29/11/2012 | | | 28 | | Click
3 | 1 | MKH05339 | | ELECTRICAL STIMULATOR, ACUPUNCTURE | test | 21/10/2012 | 24/10/2012 | | | 60 | | Click
New Borrow
1 of 1

User can add new borrow details by click at “New Borrow”, view details by click at “Borrow no.“ to view details and record Return date by “Click” in “Record Return” .

- Add new borrow details by click at “New Borrow”.

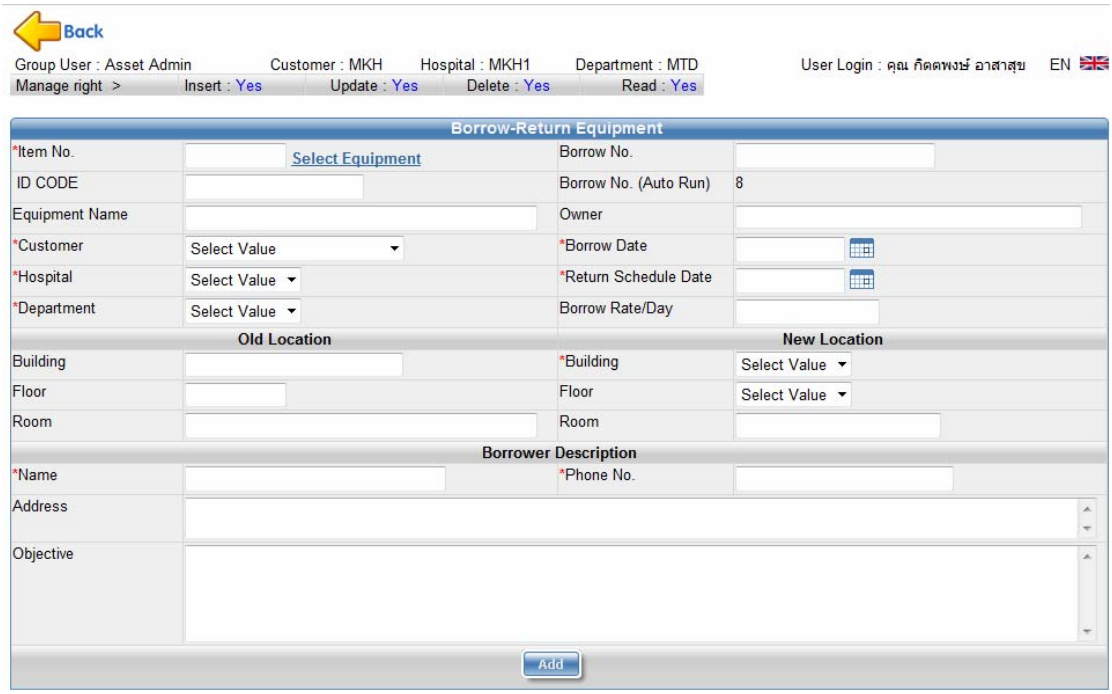

O After Add button, page for select equipment will show up and red point will appear infront of not yet return record.

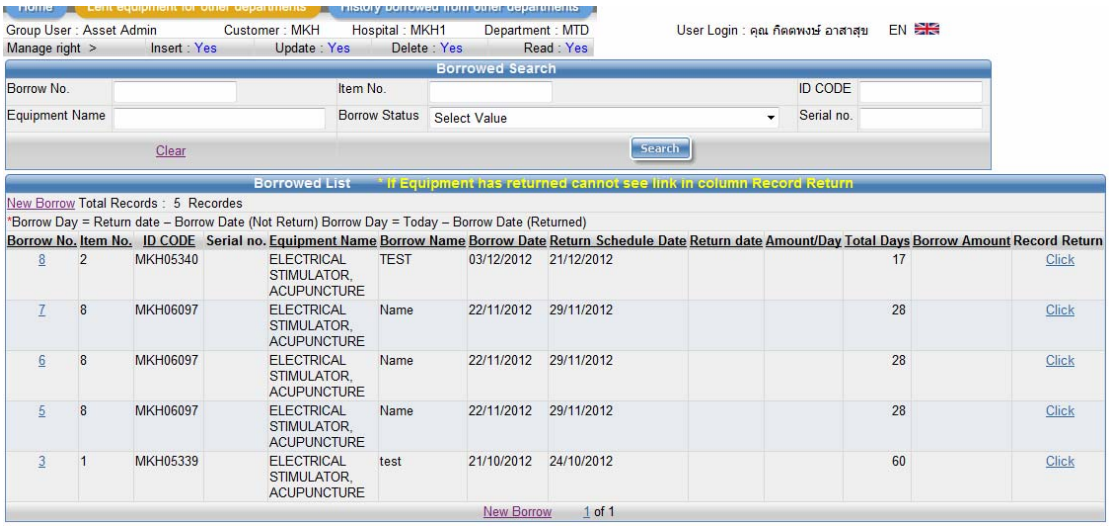
Group User : Asset Admin
Customer : MKH
Hospital : MKH1
Department : MTD
User Login : คุณ กิตตพงษ์ อาสาสุข
EN
Manage right >
Insert : Yes
Update : Yes
Delete : Yes
Read : Yes
Borrowed Search
Borrow No.
Item No.
ID CODE
Equipment Name
Borrow Status
Select Value
Serial no.
Clear
Search
Borrowed List
* If Equipment has returned cannot see link in column Record Return
New Borrow Total Records : 5 Recordes
*Borrow Day = Return date – Borrow Date (Not Return) Borrow Day = Today – Borrow Date (Returned)
Borrow No. | Item No. | ID CODE | Serial no. | Equipment Name | Borrow Name | Borrow Date | Return Schedule Date | Return date | Amount/Day | Total Days | Borrow Amount | Record Return
8 | 2 | MKH05340 | | ELECTRICAL STIMULATOR, ACUPUNCTURE | TEST | 03/12/2012 | 21/12/2012 | | | 17 | | Click
7 | 8 | MKH06097 | | ELECTRICAL STIMULATOR, ACUPUNCTURE | Name | 22/11/2012 | 29/11/2012 | | | 28 | | Click
6 | 8 | MKH06097 | | ELECTRICAL STIMULATOR, ACUPUNCTURE | Name | 22/11/2012 | 29/11/2012 | | | 28 | | Click
5 | 8 | MKH06097 | | ELECTRICAL STIMULATOR, ACUPUNCTURE | Name | 22/11/2012 | 29/11/2012 | | | 28 | | Click
3 | 1 | MKH05339 | | ELECTRICAL STIMULATOR, ACUPUNCTURE | test | 21/10/2012 | 24/10/2012 | | | 60 | | Click
New Borrow 1 of 1

➢ View borrow details by click at "# Borrow no." to view details

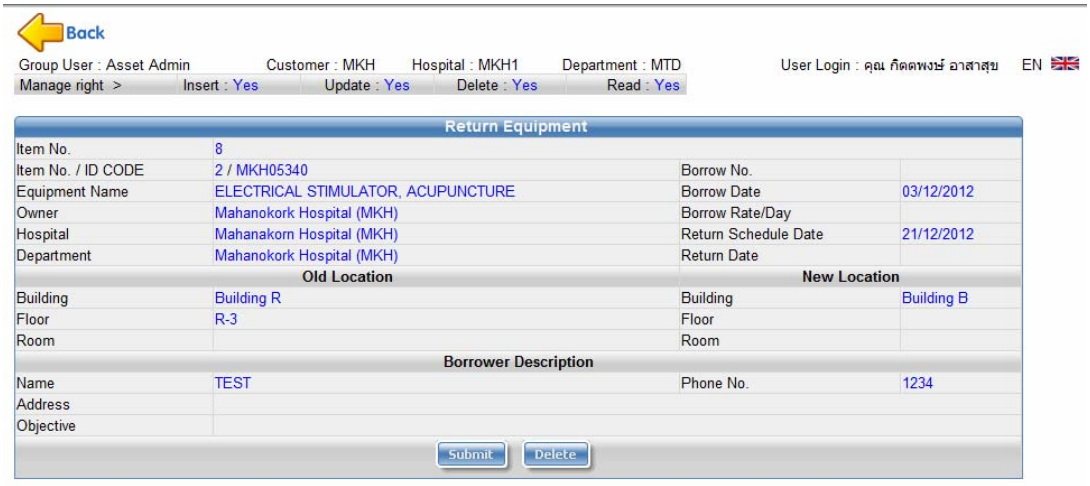

➢ Record return date, “Click” in “Record Return” column. After click in Record Return column will enter to Return Equipment page.

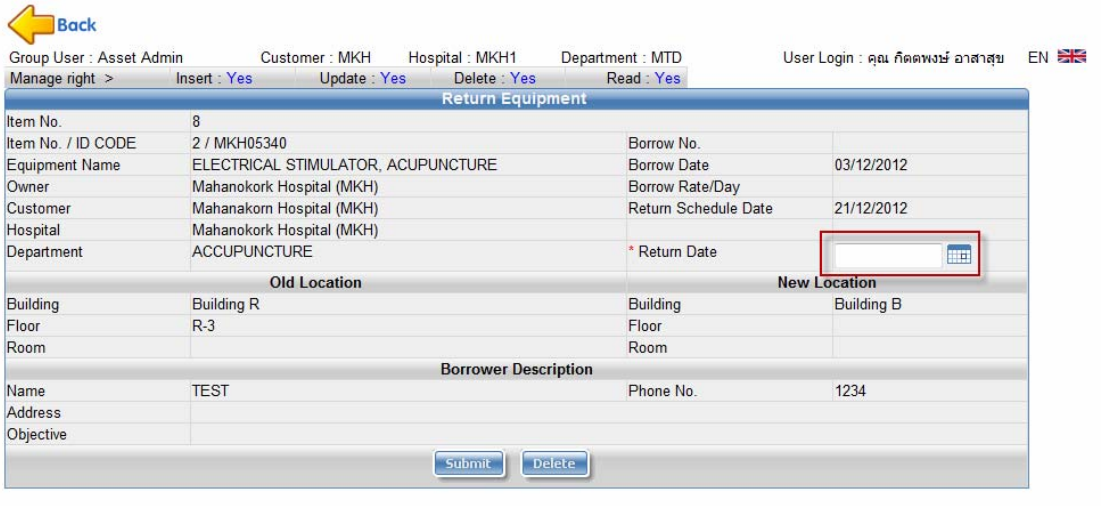

Transfer

Transfer

For equipment owner department record equipment transfer for record history. Transference also process in monthly examine equipment. If transfer to other department without record, user need to record transference and after record owner will be changed in suddenly. Request, PM, CAL details will move to new owner department.

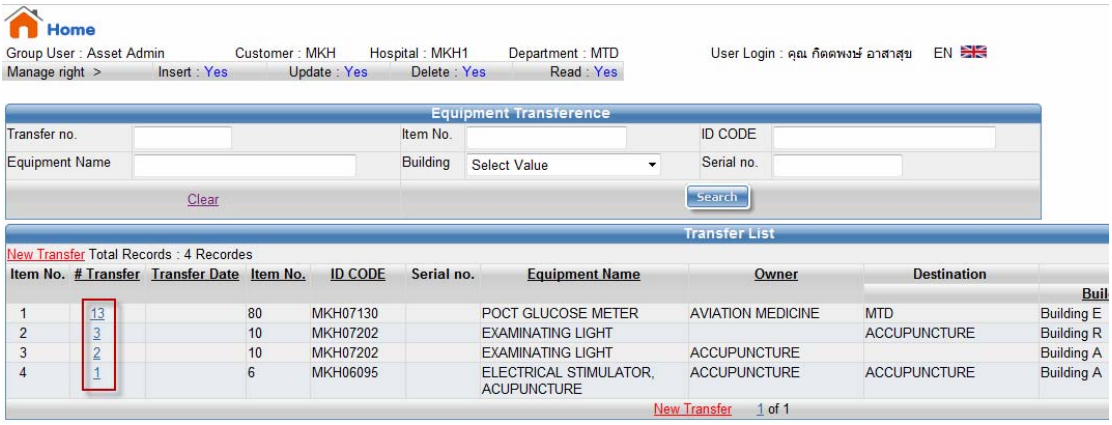
Home
Group User : Asset Admin
Customer : MKH
Hospital : MKH1
Department : MTD
User Login : คุณ กิตตพงษ์ อาสาสุข
EN
Manage right >
Insert : Yes
Update : Yes
Delete : Yes
Read : Yes
Equipment Transference
Transfer no.
Item No.
ID CODE
Equipment Name
Building
Select Value
Serial no.
Clear
Search
Transfer List
New Transfer Total Records : 4 Recordes
Item No. # Transfer Transfer Date Item No. ID CODE Serial no. Equipment Name Owner Destination
1 13 80 MKH07130 POCT GLUCOSE METER AVIATION MEDICINE MTD Building E
2 3 10 MKH07202 EXAMINATING LIGHT ACCUPUNCTURE Building R
3 2 10 MKH07202 EXAMINATING LIGHT ACCUPUNCTURE Building A
4 1 6 MKH06095 ELECTRICAL STIMULATOR, ACUPUNCTURE ACCUPUNCTURE ACCUPUNCTURE Building A
New Transfer 1 of 1

User can add transfer details by click at "New Transfer" and view transfer details by click at "# Tranfer" to view details.

Transference can transfer only in hospital in same network.

➢ Add transfer details by click at "New Transfer".

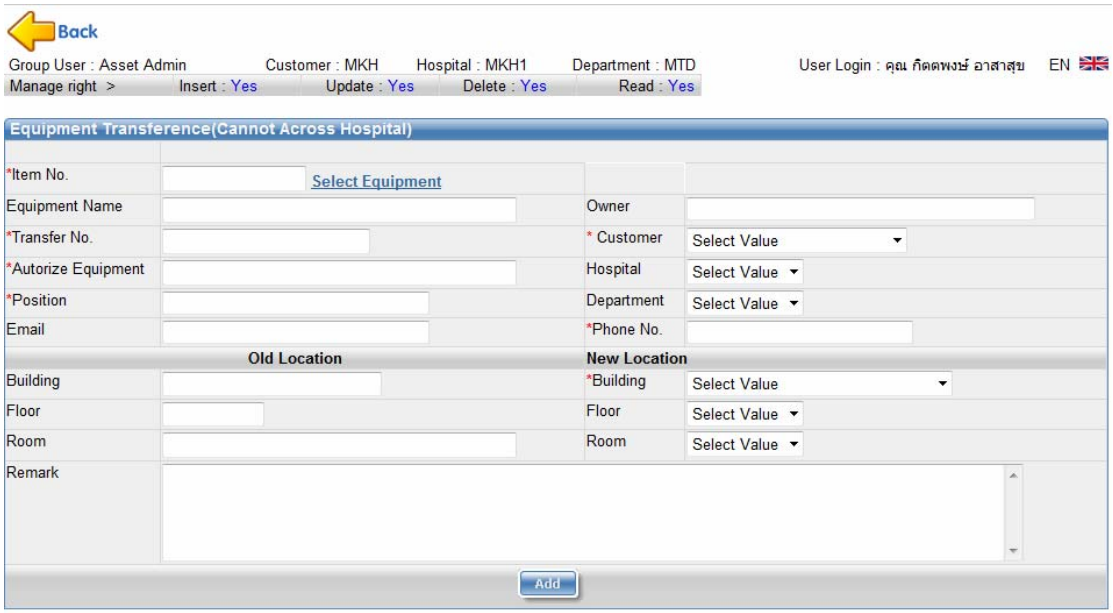

➢ View Transference details by click at "# Transfer" to view details.

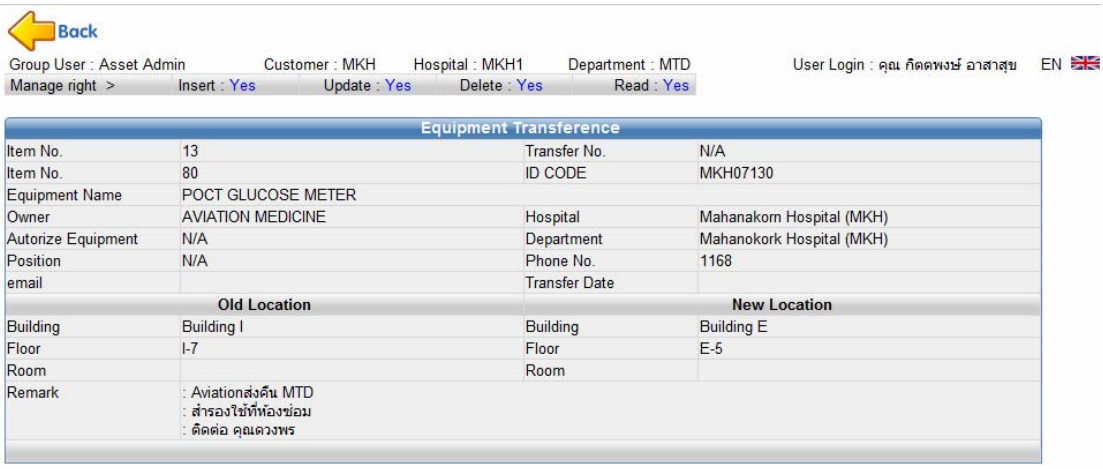

Move Location

Move Location

For record moving location of equipment to building, floor, new room but same owner department.

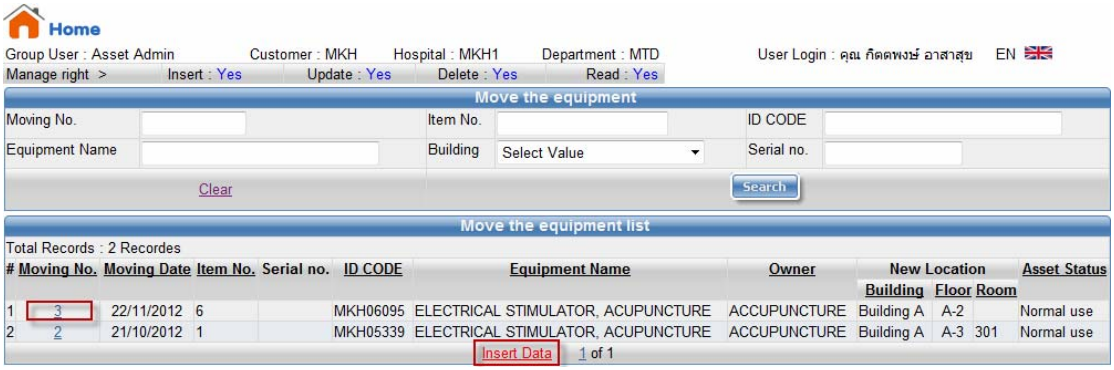
Home
Group User : Asset Admin
Customer : MKH
Hospital : MKH1
Department : MTD
User Login : คุณ กิตตพงษ์ อาสาสุข
EN
Manage right >
Insert : Yes
Update : Yes
Delete : Yes
Read : Yes
Move the equipment
Moving No.
Item No.
ID CODE
Equipment Name
Building
Select Value
Serial no.
Clear
Search
Move the equipment list
Total Records : 2 Recordes
Moving No. Moving Date Item No. Serial no. ID CODE Equipment Name Owner New Location Asset Status
Building Floor Room
1 3 22/11/2012 6 MKH06095 ELECTRICAL STIMULATOR, ACUPUNCTURE ACCUPUNCTURE Building A A-2 Normal use
2 2 21/10/2012 1 MKH05339 ELECTRICAL STIMULATOR, ACUPUNCTURE ACCUPUNCTURE Building A A-3 301 Normal use
Insert Data
1 of 1

Use can add moving details by click at "Insert data" and view details ny click at "No." that want to view details.

➢ Add move location details by click at "Insert data".

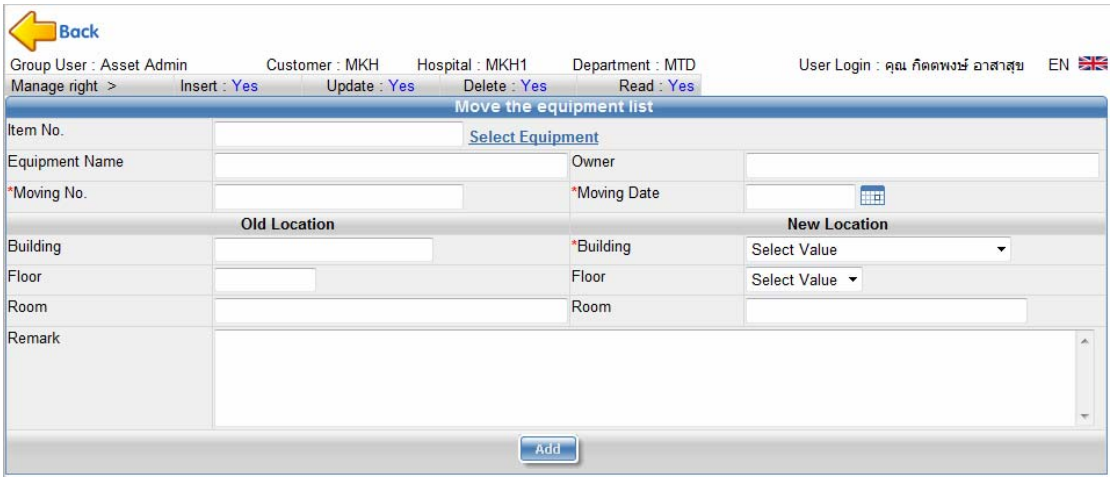

➢ View move location details by click at “Moving no.” .

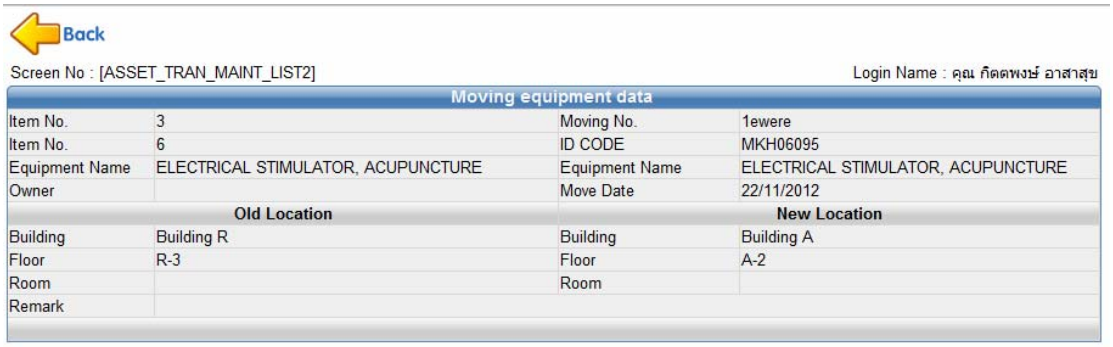
Back
Screen No : [ASSET_TRAN_MAINT_LIST2]
Login Name : คุณ กิตตพงษ์ อาสาสุข
Moving equipment data
Item No. 3 Moving No. 1ewere
Item No. 6 ID CODE MKH06095
Equipment Name ELECTRICAL STIMULATOR, ACUPUNCTURE Equipment Name ELECTRICAL STIMULATOR, ACUPUNCTURE
Owner Move Date 22/11/2012
Old Location New Location
Building Building R Building Building A
Floor R-3 Floor A-2
Room Room
Remark

Calculate depreciation

Calculate depreciation.

To calculate depreciation system will calculate depreciation of all equipment records in system by Straight-Line Depreciation Method. Data to use for calaulate is calculate depreciation start date, purchase price, quantity of working year and scrap value.

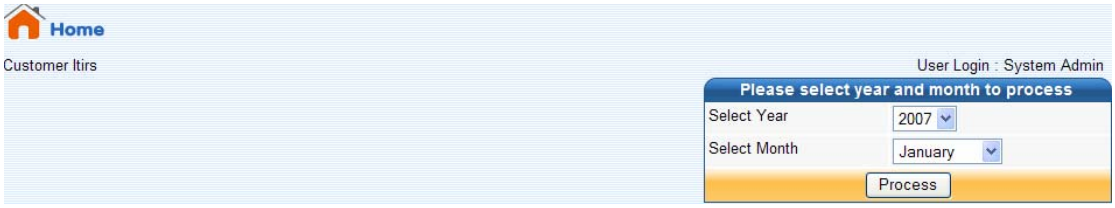

Procession will calculate at the end of every month. To select data to calculate select from :

- Select year Click to select year that need to calculate.
- Select month Click to select month that need to calculate.

Select year and month to calculate and click “Process” button.

After process system will warn completed process and record each equipment calculation.

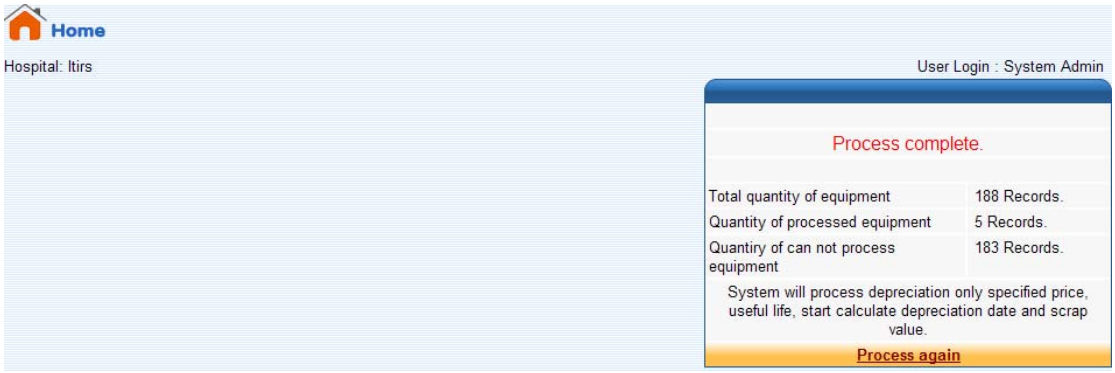
Home
Hospital: Itirs
User Login : System Admin
Process complete.
Total quantity of equipment 188 Records.
Quantity of processed equipment 5 Records.
Quantiry of can not process equipment 183 Records.
System will process depreciation only specified price, useful life, start calculate depreciation date and scrap value.
Process again

Export Data

Over view

Export data to Excel for easy to take public information to use with other system or use for working. System prepared export data to excel divied in 3 parts follow as below.

1. Cost of repair
2. Equipment Date
3. Export Equipment Template Excel

Logged in department will see only own department's data but for Asset Admin group will all department in hospital group.

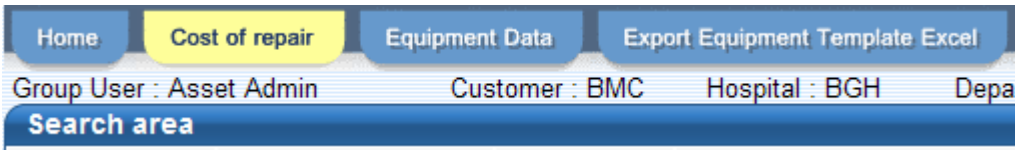

Cost of repair

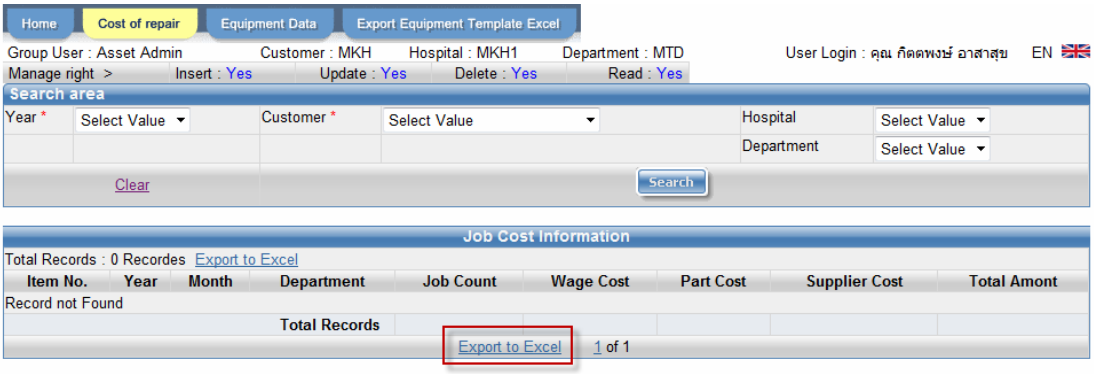

User have to select year to Export data and click at "Export to Excel" . Wait for a sec. warning popup for open to view file or save file will appear.

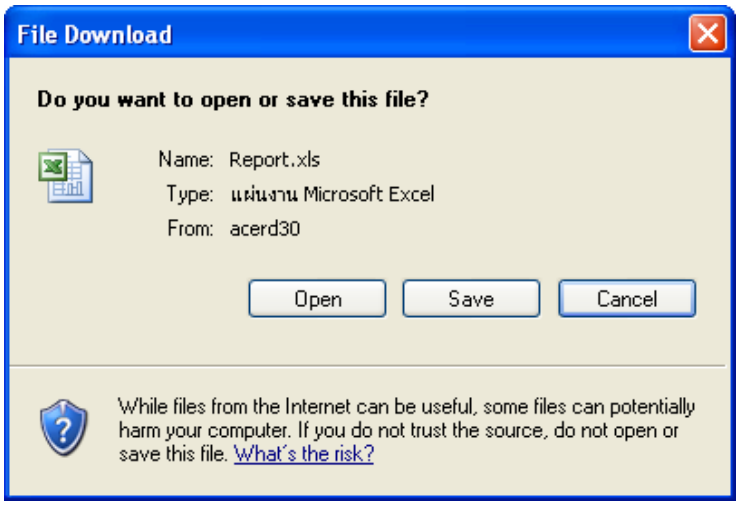
File Download
Do you want to open or save this file?
Name: Report.xls
Type: แผ่นงาน Microsoft Excel
From: acerd30
Open
Save
Cancel
While files from the Internet can be useful, some files can potentially harm your computer. If you do not trust the source, do not open or save this file. What's the risk?

If user want to open to view Excel File click at Open. If user want to save file click Save and select file location to save, user can Rename excel file from Export.

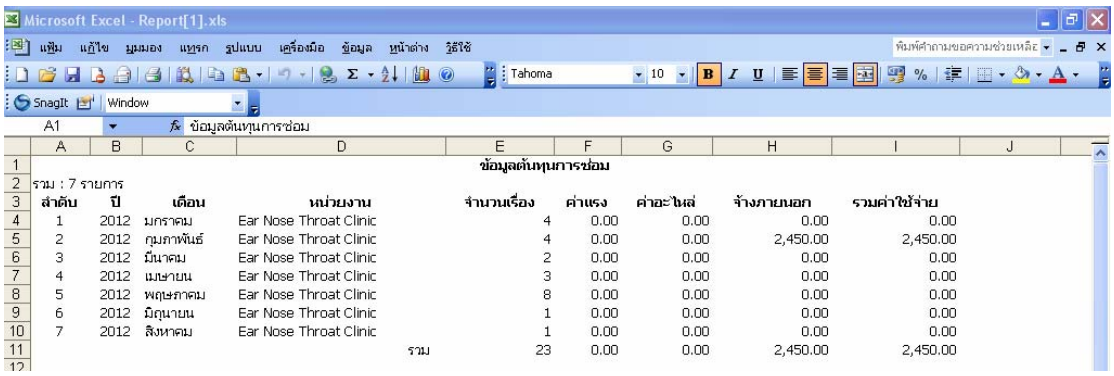

Microsoft Excel - Report[1].xls

ข้อมูลต้นทุนการซ่อม

รวม : 7 รายการ

ลำดับ	ปี	เดือน	หน่วยงาน	จำนวนเรื่อง	ค่าแรง	ค่าอะไหล่	จ้างภายนอก	รวมค่าใช้จ่าย
1	2012	มกราคม	Ear Nose Throat Clinic	4	0.00	0.00	0.00	0.00
2	2012	กุมภาพันธ์	Ear Nose Throat Clinic	4	0.00	0.00	2,450.00	2,450.00
3	2012	มีนาคม	Ear Nose Throat Clinic	2	0.00	0.00	0.00	0.00
4	2012	เมษายน	Ear Nose Throat Clinic	3	0.00	0.00	0.00	0.00
5	2012	พฤษภาคม	Ear Nose Throat Clinic	8	0.00	0.00	0.00	0.00
6	2012	มิถุนายน	Ear Nose Throat Clinic	1	0.00	0.00	0.00	0.00
7	2012	สิงหาคม	Ear Nose Throat Clinic	1	0.00	0.00	0.00	0.00
			รวม	23	0.00	0.00	2,450.00	2,450.00

Equipment Data.

Select customer in Search area.

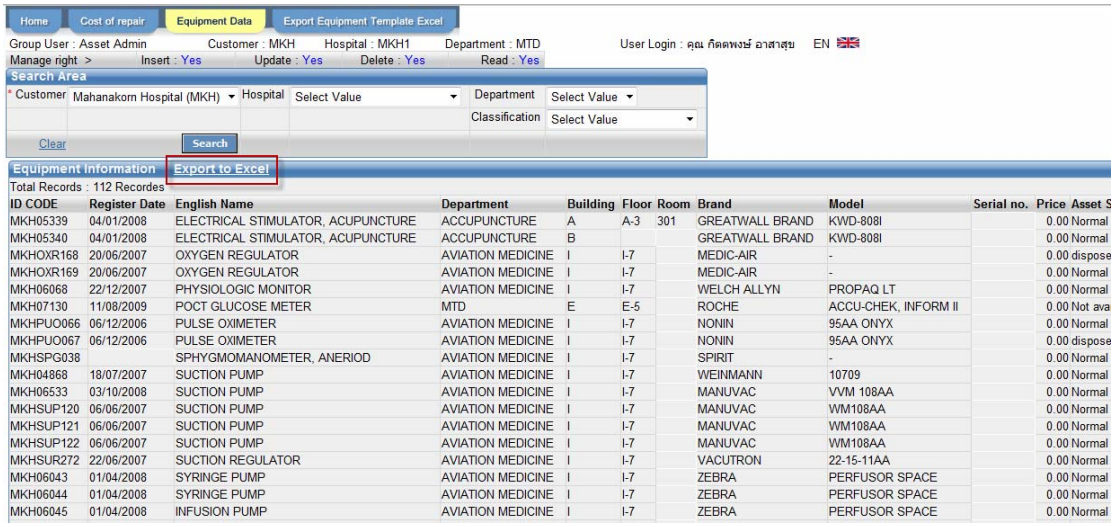

Home | Cost of repair | Equipment Data | Export Equipment Template Excel

Group User : Asset Admin Customer : MKH Hospital : MKH1 Department : MTD User Login : คุณ กิตตพงษ์ อาสาสุข EN

Manage right > Insert : Yes Update : Yes Delete : Yes Read : Yes

Search Area

* Customer: Mahanakorn Hospital (MKH) Hospital: Select Value Department: Select Value Classification: Select Value

Clear Search

Equipment Information Export to Excel

Total Records : 112 Recordes

ID CODE	Register Date	English Name	Department	Building	Floor	Room	Brand	Model	Serial no.	Price	Asset S
MKH05339	04/01/2008	ELECTRICAL STIMULATOR, ACUPUNCTURE	ACCUPUNCTURE	A	A-3	301	GREATWALL BRAND	KWD-808I		0.00	Normal
MKH05340	04/01/2008	ELECTRICAL STIMULATOR, ACUPUNCTURE	ACCUPUNCTURE	B			GREATWALL BRAND	KWD-808I		0.00	Normal
MKHOXR168	20/06/2007	OXYGEN REGULATOR	AVIATION MEDICINE	I	I-7		MEDIC-AIR	-		0.00	dispose
MKHOXR169	20/06/2007	OXYGEN REGULATOR	AVIATION MEDICINE	I	I-7		MEDIC-AIR	-		0.00	Normal
MKH06068	22/12/2007	PHYSIOLOGIC MONITOR	AVIATION MEDICINE	I	I-7		WELCH ALLYN	PROPAQ LT		0.00	Normal
MKH07130	11/08/2009	POCT GLUCOSE METER	MTD	E	E-5		ROCHE	ACCU-CHEK, INFORM II		0.00	Not ava
MKHPUO066	06/12/2006	PULSE OXIMETER	AVIATION MEDICINE	I	I-7		NONIN	95AA ONYX		0.00	Normal
MKHPUO067	06/12/2006	PULSE OXIMETER	AVIATION MEDICINE	I	I-7		NONIN	95AA ONYX		0.00	dispose
MKHSPG038		SPHYGMOMANOMETER, ANERIOD	AVIATION MEDICINE	I	I-7		SPIRIT	-		0.00	Normal
MKH04868	18/07/2007	SUCTION PUMP	AVIATION MEDICINE	I	I-7		WEINMANN	10709		0.00	Normal
MKH06533	03/10/2008	SUCTION PUMP	AVIATION MEDICINE	I	I-7		MANUVAC	VVM 108AA		0.00	Normal
MKHSUP120	06/06/2007	SUCTION PUMP	AVIATION MEDICINE	I	I-7		MANUVAC	WM108AA		0.00	Normal
MKHSUP121	06/06/2007	SUCTION PUMP	AVIATION MEDICINE	I	I-7		MANUVAC	WM108AA		0.00	Normal
MKHSUP122	06/06/2007	SUCTION PUMP	AVIATION MEDICINE	I	I-7		MANUVAC	WM108AA		0.00	Normal
MKHSUR272	22/06/2007	SUCTION REGULATOR	AVIATION MEDICINE	I	I-7		VACUTRON	22-15-11AA		0.00	Normal
MKH06043	01/04/2008	SYRINGE PUMP	AVIATION MEDICINE	I	I-7		ZEBRA	PERFUSOR SPACE		0.00	Normal
MKH06044	01/04/2008	SYRINGE PUMP	AVIATION MEDICINE	I	I-7		ZEBRA	PERFUSOR SPACE		0.00	Normal
MKH06045	01/04/2008	INFUSION PUMP	AVIATION MEDICINE	I	I-7		ZEBRA	PERFUSOR SPACE		0.00	Normal

Click at Export to Excel wait for a while popup will appear.

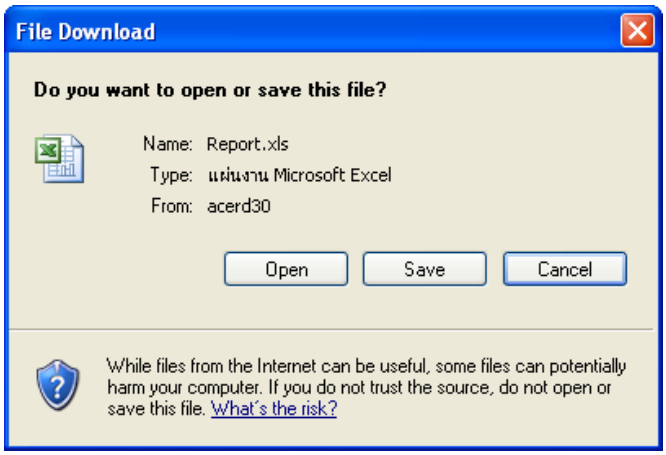
File Download
Do you want to open or save this file?
Name: Report.xls
Type: แผ่นงาน Microsoft Excel
From: acerd30
Open
Save
Cancel
While files from the Internet can be useful, some files can potentially harm your computer. If you do not trust the source, do not open or save this file. What's the risk?

Export Equipment Template Excel.

Select customer.

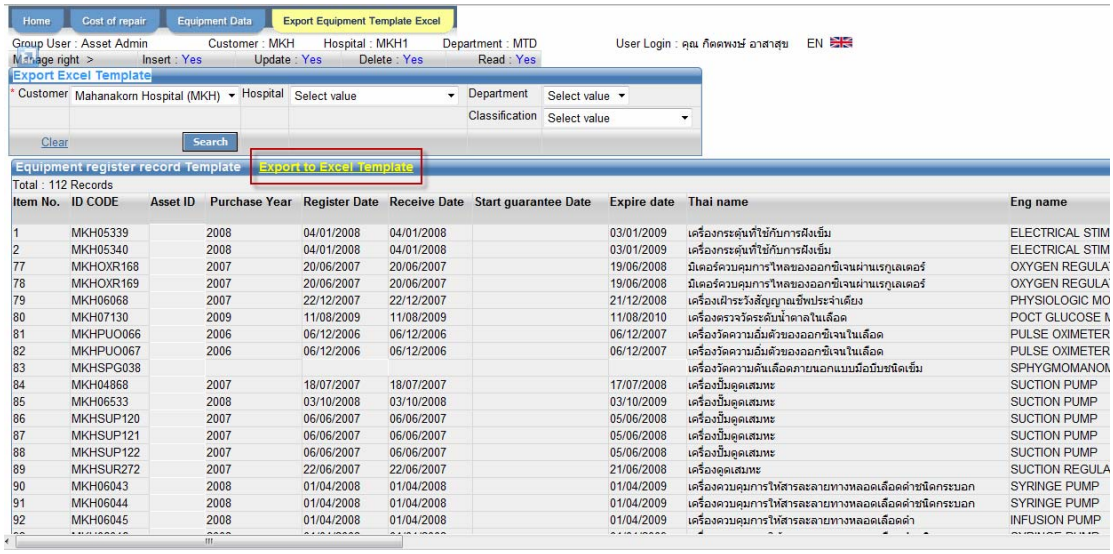

Item No.	ID CODE	Asset ID	Purchase Year	Register Date	Receive Date	Start guarantee Date	Expire date	Thai name	Eng name
1	MKH05339		2008	04/01/2008	04/01/2008		03/01/2009	เครื่องกระตุ้นที่ใช้กับการฝังเข็ม	ELECTRICAL STIM
2	MKH05340		2008	04/01/2008	04/01/2008		03/01/2009	เครื่องกระตุ้นที่ใช้กับการฝังเข็ม	ELECTRICAL STIM
77	MKHOXR168		2007	20/06/2007	20/06/2007		19/06/2008	มิเตอร์ควบคุมการไหลของออกซิเจนผ่านเรกูเลเตอร์	OXYGEN REGULA
78	MKHOXR169		2007	20/06/2007	20/06/2007		19/06/2008	มิเตอร์ควบคุมการไหลของออกซิเจนผ่านเรกูเลเตอร์	OXYGEN REGULA
79	MKH06068		2007	22/12/2007	22/12/2007		21/12/2008	เครื่องเฝ้าระวังสัญญาณชีพประจำเตียง	PHYSIOLOGIC MO
80	MKH07130		2009	11/08/2009	11/08/2009		11/08/2010	เครื่องตรวจวัดระดับน้ำตาลในเลือด	POCT GLUCOSE M
81	MKHPUO066		2006	06/12/2006	06/12/2006		06/12/2007	เครื่องวัดความอิ่มตัวของออกซิเจนในเลือด	PULSE OXIMETER
82	MKHPUO067		2006	06/12/2006	06/12/2006		06/12/2007	เครื่องวัดความอิ่มตัวของออกซิเจนในเลือด	PULSE OXIMETER
83	MKHSPG038							เครื่องวัดความดันเลือดภายนอกแบบมือบีบชนิดเข็ม	SPHYGMOMANOM
84	MKH04868		2007	18/07/2007	18/07/2007		17/07/2008	เครื่องปั๊มดูดเสมหะ	SUCTION PUMP
85	MKH06533		2008	03/10/2008	03/10/2008		03/10/2009	เครื่องปั๊มดูดเสมหะ	SUCTION PUMP
86	MKHSUP120		2007	06/06/2007	06/06/2007		05/06/2008	เครื่องปั๊มดูดเสมหะ	SUCTION PUMP
87	MKHSUP121		2007	06/06/2007	06/06/2007		05/06/2008	เครื่องปั๊มดูดเสมหะ	SUCTION PUMP
88	MKHSUP122		2007	06/06/2007	06/06/2007		05/06/2008	เครื่องปั๊มดูดเสมหะ	SUCTION PUMP
89	MKHSUR272		2007	22/06/2007	22/06/2007		21/06/2008	เครื่องดูดเสมหะ	SUCTION REGULA
90	MKH06043		2008	01/04/2008	01/04/2008		01/04/2009	เครื่องควบคุมการให้สารละลายทางหลอดเลือดด่าชนิดกระบอก	SYRINGE PUMP
91	MKH06044		2008	01/04/2008	01/04/2008		01/04/2009	เครื่องควบคุมการให้สารละลายทางหลอดเลือดด่าชนิดกระบอก	SYRINGE PUMP
92	MKH06045		2008	01/04/2008	01/04/2008		01/04/2009	เครื่องควบคุมการให้สารละลายทางหลอดเลือดด่า	INFUSION PUMP

Click at Export to Excel wait for a while warning popup to open or save file will appear.

Dispose equipment

Dispose equipment

For search equipment record which should be dispose, details follow as below.

- Equipment should be dispose.
- Equipment should be dispose by technicians comment.
- Disposed equipment.

Equipment should be dispose

Asset Admin has duty to manage equipment, which should be dispose by join with owner of equipment that should be dispose or not. Considering from useful life, accumulate of repair cost percentage compare with purchase price. For any equipement should be dispose will report to authori to approve, when approved then record dispose details. Disposed record can not request repair, PM and CAL.

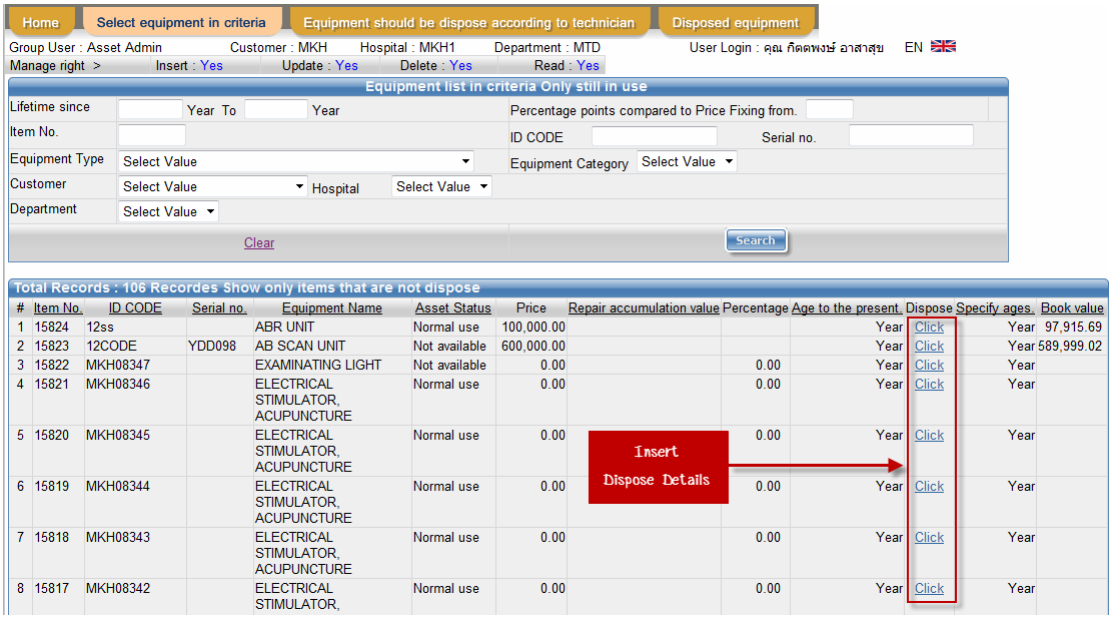
Home
Select equipment in criteria
Equipment should be dispose according to technician
Disposed equipment
Group User : Asset Admin
Customer : MKH
Hospital : MKH1
Department : MTD
User Login : คุณ กิตติพงษ์ อาสาสุข
EN
Manage right >
Insert : Yes
Update : Yes
Delete : Yes
Read : Yes
Equipment list in criteria Only still in use
Lifetime since
Year To
Year
Percentage points compared to Price Fixing from.
Item No.
ID CODE
Serial no.
Equipment Type
Select Value
Equipment Category
Select Value
Customer
Select Value
Hospital
Select Value
Department
Select Value
Clear
Search
Total Records : 106 Recordes Show only items that are not dispose
Item No. ID CODE Serial no. Equipment Name Asset Status Price Repair accumulation value Percentage Age to the present. Dispose Specify ages. Book value
1 15824 12ss ABR UNIT Normal use 100,000.00 Year Click Year 97,915.69
2 15823 12CODE YDD098 AB SCAN UNIT Not available 600,000.00 Year Click Year 589,999.02
3 15822 MKH08347 EXAMINATING LIGHT Not available 0.00 0.00 Year Click Year
4 15821 MKH08346 ELECTRICAL STIMULATOR, ACUPUNCTURE Normal use 0.00 0.00 Year Click Year
5 15820 MKH08345 ELECTRICAL STIMULATOR, ACUPUNCTURE Normal use 0.00 0.00 Year Click Year
6 15819 MKH08344 ELECTRICAL STIMULATOR, ACUPUNCTURE Normal use 0.00 0.00 Year Click Year
7 15818 MKH08343 ELECTRICAL STIMULATOR, ACUPUNCTURE Normal use 0.00 0.00 Year Click Year
8 15817 MKH08342 ELECTRICAL STIMULATOR, Normal use 0.00 0.00 Year Click Year
Insert
Dispose Details

- Click in Dispose column to insert dispose details.

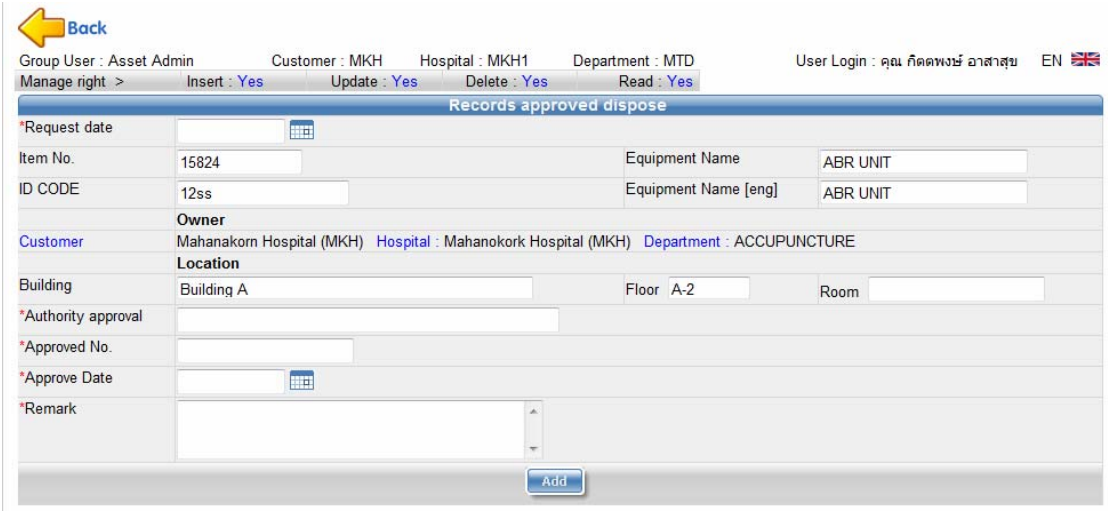

Equipment should be dispose by technician's comment.

Although this case does not comply with the standard. If technician's comment is not worth to repair, status in repair order will be Dispose and this record will appear in this page for Asset admid approve for dispose, after approved user need to record dispose in this page.

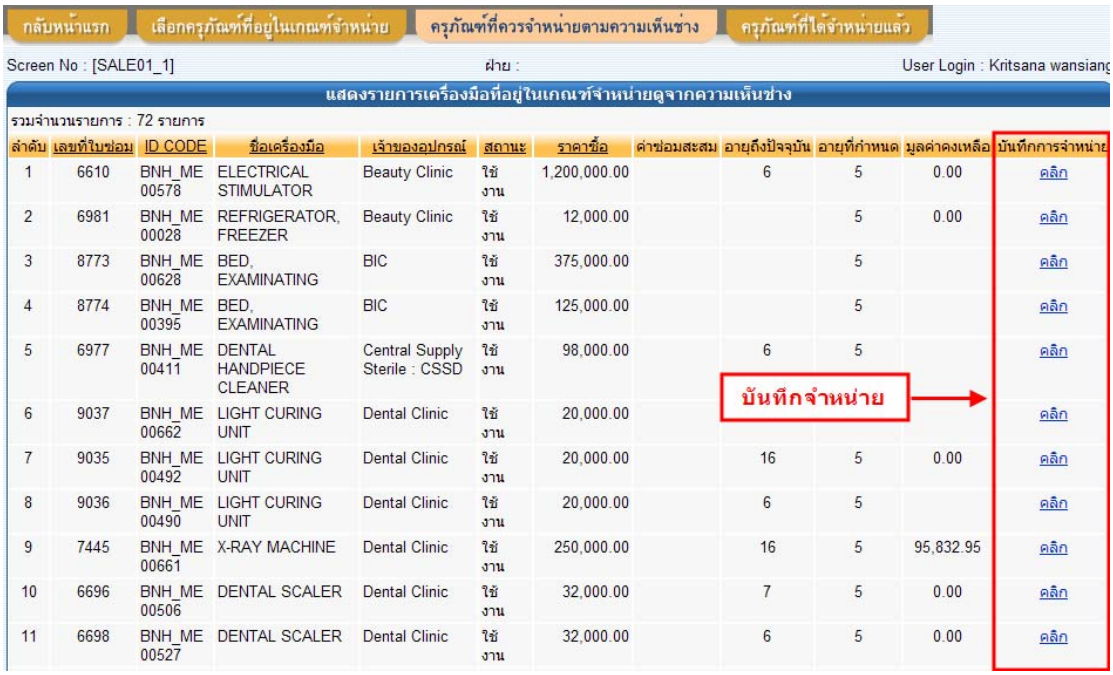
กลับหน้าแรก
เลือกครุภัณฑ์ที่อยู่ในเกณฑ์จำหน่าย
ครุภัณฑ์ที่ควรจำหน่ายตามความเห็นช่าง
ครุภัณฑ์ที่ได้จำหน่ายแล้ว
Screen No : [SALE01_1]
ฝ่าย :
User Login : Kritsana wansiang
แสดงรายการเครื่องมือที่อยู่ในเกณฑ์จำหน่ายดูจากความเห็นช่าง
รวมจำนวนรายการ : 72 รายการ
ลำดับ | เลขที่ใบซ่อม | ID CODE | ชื่อเครื่องมือ | เจ้าของอุปกรณ์ | สถานะ | ราคาซื้อ | ค่าซ่อมสะสม | อายุถึงปัจจุบัน | อายุที่กำหนด | มูลค่าคงเหลือ | บันทึกการจำหน่าย
1 | 6610 | BNH_ME 00578 | ELECTRICAL STIMULATOR | Beauty Clinic | ใช้งาน | 1,200,000.00 | | 6 | 5 | 0.00 | คลิก
2 | 6981 | BNH_ME 00028 | REFRIGERATOR, FREEZER | Beauty Clinic | ใช้งาน | 12,000.00 | | | 5 | 0.00 | คลิก
3 | 8773 | BNH_ME 00628 | BED, EXAMINATING | BIC | ใช้งาน | 375,000.00 | | | 5 | | คลิก
4 | 8774 | BNH_ME 00395 | BED, EXAMINATING | BIC | ใช้งาน | 125,000.00 | | | 5 | | คลิก
5 | 6977 | BNH_ME 00411 | DENTAL HANDPIECE CLEANER | Central Supply Sterile : CSSD | ใช้งาน | 98,000.00 | | 6 | 5 | | คลิก
6 | 9037 | BNH_ME 00662 | LIGHT CURING UNIT | Dental Clinic | ใช้งาน | 20,000.00 | | | | | คลิก
7 | 9035 | BNH_ME 00492 | LIGHT CURING UNIT | Dental Clinic | ใช้งาน | 20,000.00 | | 16 | 5 | 0.00 | คลิก
8 | 9036 | BNH_ME 00490 | LIGHT CURING UNIT | Dental Clinic | ใช้งาน | 20,000.00 | | 6 | 5 | | คลิก
9 | 7445 | BNH_ME 00661 | X-RAY MACHINE | Dental Clinic | ใช้งาน | 250,000.00 | | 16 | 5 | 95,832.95 | คลิก
10 | 6696 | BNH_ME 00506 | DENTAL SCALER | Dental Clinic | ใช้งาน | 32,000.00 | | 7 | 5 | 0.00 | คลิก
11 | 6698 | BNH_ME 00527 | DENTAL SCALER | Dental Clinic | ใช้งาน | 32,000.00 | | 6 | 5 | 0.00 | คลิก
บันทึกจำหน่าย

- Click Dispose to insert dispose details.

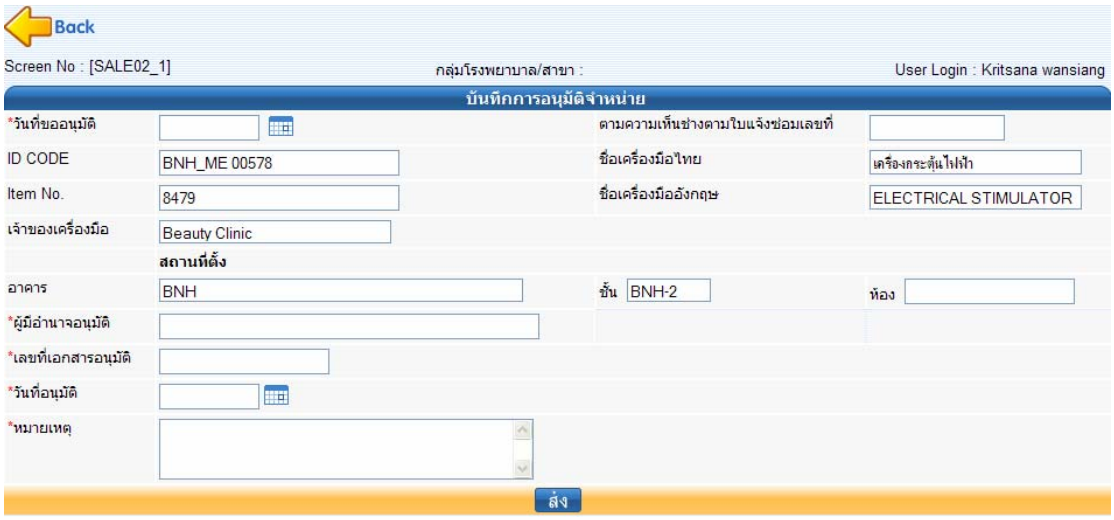

Disposed equipment

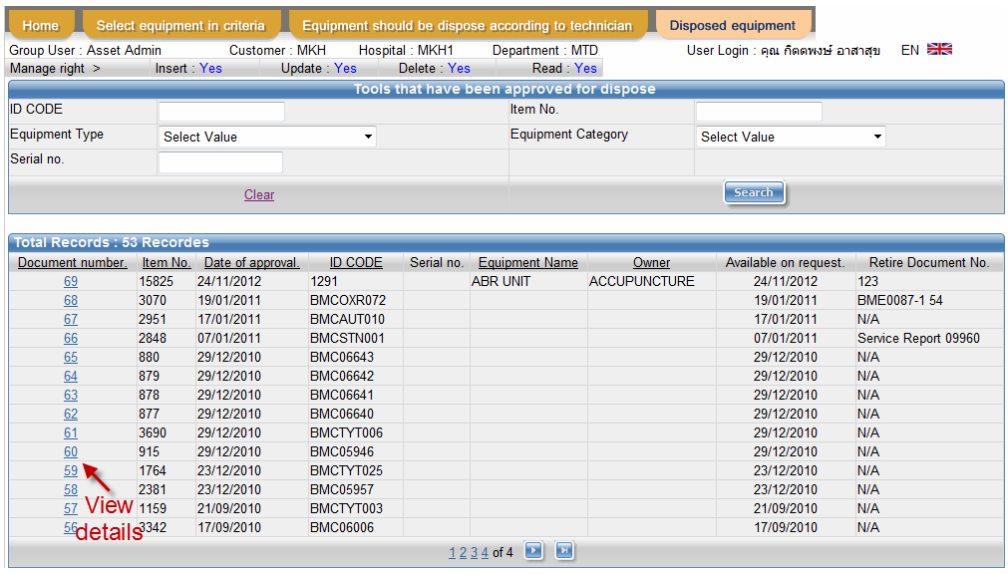

- Click #Document to view dispose details.

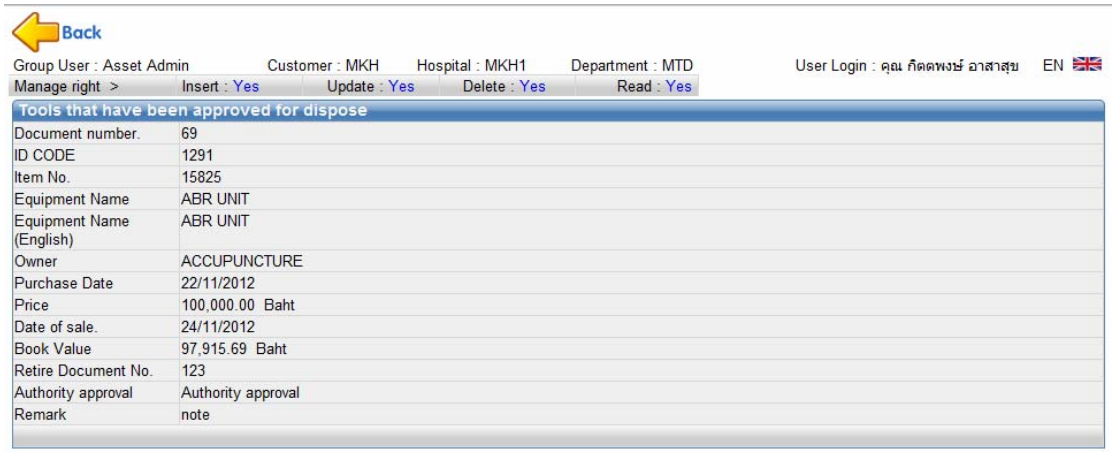

Print Label

Print Label

Logged in department able to select print equipment label to A4 size sticker paper for own department to stick on equipment.

- Select equipment to print label by tick in checkbox on the right side and scroll to the bottom to save.

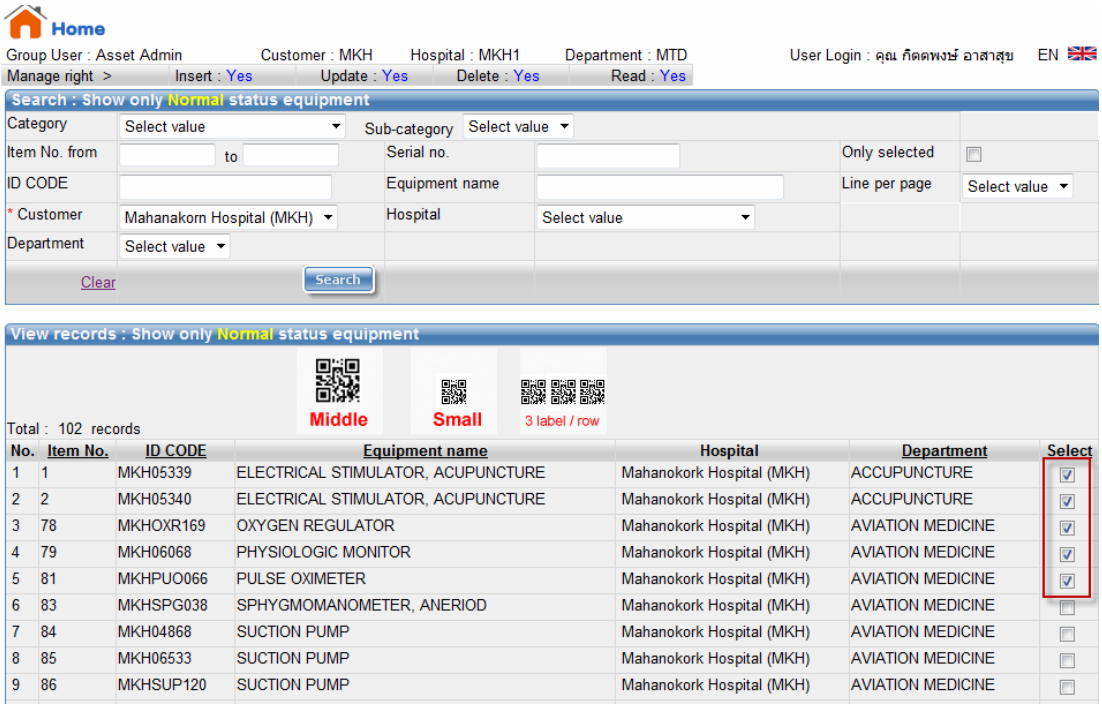
Home
Group User : Asset Admin
Customer : MKH
Hospital : MKH1
Department : MTD
User Login : คุณ กิตตพงษ์ อาสาสุข
EN
Manage right >
Insert : Yes
Update : Yes
Delete : Yes
Read : Yes
Search : Show only Normal status equipment
Category
Select value
Sub-category
Select value
Item No. from
to
Serial no.
Only selected
ID CODE
Equipment name
Line per page
Select value
* Customer
Mahanakorn Hospital (MKH)
Hospital
Select value
Department
Select value
Clear
Search
View records : Show only Normal status equipment
Middle
Small
3 label / row
Total : 102 records
No. Item No. ID CODE Equipment name Hospital Department Select
1 1 MKH05339 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
2 2 MKH05340 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
3 78 MKHOXR169 OXYGEN REGULATOR Mahanokork Hospital (MKH) AVIATION MEDICINE
4 79 MKH06068 PHYSIOLOGIC MONITOR Mahanokork Hospital (MKH) AVIATION MEDICINE
5 81 MKHPUO066 PULSE OXIMETER Mahanokork Hospital (MKH) AVIATION MEDICINE
6 83 MKHSPG038 SPHYGMOMANOMETER, ANERIOD Mahanokork Hospital (MKH) AVIATION MEDICINE
7 84 MKH04868 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
8 85 MKH06533 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
9 86 MKHSUP120 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE

- Save.
- Click Print Label button.

Print Label

Logged in department able to select print equipment label to sticker paper for own department to stick on equipment.

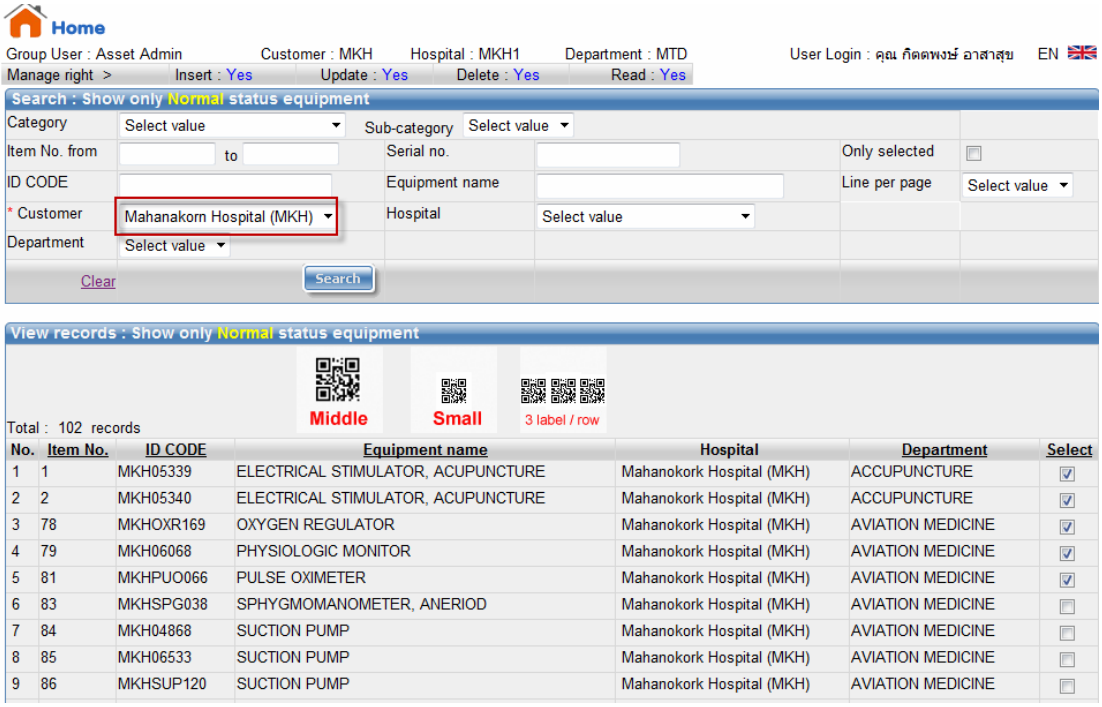
Home
Group User : Asset Admin
Customer : MKH
Hospital : MKH1
Department : MTD
User Login : คุณ กิตพงษ์ อาสาสุข
EN
Manage right >
Insert : Yes
Update : Yes
Delete : Yes
Read : Yes
Search : Show only Normal status equipment
Category
Select value
Sub-category
Select value
Item No. from
to
Serial no.
Only selected
ID CODE
Equipment name
Line per page
Select value
* Customer
Mahanakorn Hospital (MKH)
Hospital
Select value
Department
Select value
Clear
Search
View records : Show only Normal status equipment
Middle
Small
3 label / row
Total : 102 records
No. Item No. ID CODE Equipment name Hospital Department Select
1 1 MKH05339 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
2 2 MKH05340 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
3 78 MKHOXR169 OXYGEN REGULATOR Mahanokork Hospital (MKH) AVIATION MEDICINE
4 79 MKH06068 PHYSIOLOGIC MONITOR Mahanokork Hospital (MKH) AVIATION MEDICINE
5 81 MKHPUO066 PULSE OXIMETER Mahanokork Hospital (MKH) AVIATION MEDICINE
6 83 MKHSPG038 SPHYGMOMANOMETER, ANERIOD Mahanokork Hospital (MKH) AVIATION MEDICINE
7 84 MKH04868 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
8 85 MKH06533 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
9 86 MKHSUP120 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE

Select customer and click “Search” button will see all hospital’s equipment records. The process is as follow.

1. Clear old default (If value was specified) for select new value. System will take all of tick in checkbox out.

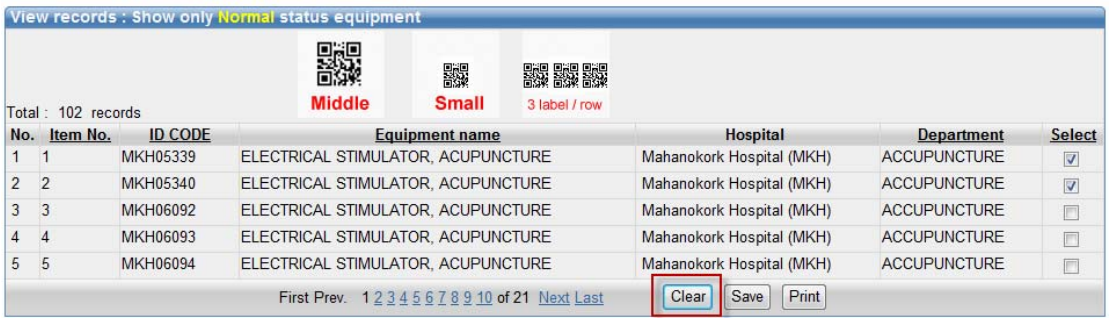
View records : Show only Normal status equipment
Middle
Small
3 label / row
Total : 102 records
No. Item No. ID CODE Equipment name Hospital Department Select
1 1 MKH05339 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
2 2 MKH05340 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
3 3 MKH06092 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
4 4 MKH06093 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
5 5 MKH06094 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
First Prev. 1 2 3 4 5 6 7 8 9 10 of 21 Next Last
Clear
Save
Print

2. Select equipment to print by tick in checkbox on the right side and scroll to the bottom for save.

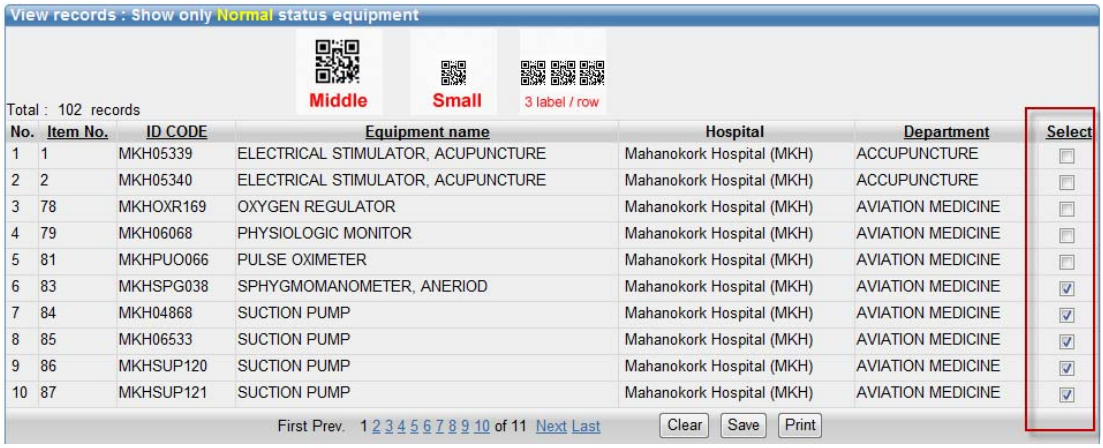
View records : Show only Normal status equipment
Middle
Small
3 label / row
Total : 102 records
No. Item No. ID CODE Equipment name Hospital Department Select
1 1 MKH05339 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
2 2 MKH05340 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
3 78 MKHOXR169 OXYGEN REGULATOR Mahanokork Hospital (MKH) AVIATION MEDICINE
4 79 MKH06068 PHYSIOLOGIC MONITOR Mahanokork Hospital (MKH) AVIATION MEDICINE
5 81 MKHPUO066 PULSE OXIMETER Mahanokork Hospital (MKH) AVIATION MEDICINE
6 83 MKHSPG038 SPHYGMOMANOMETER, ANERIOD Mahanokork Hospital (MKH) AVIATION MEDICINE
7 84 MKH04868 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
8 85 MKH06533 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
9 86 MKHSUP120 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
10 87 MKHSUP121 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
First Prev. 1 2 3 4 5 6 7 8 9 10 of 11 Next Last
Clear
Save
Print

3. Sae selection (Click save).

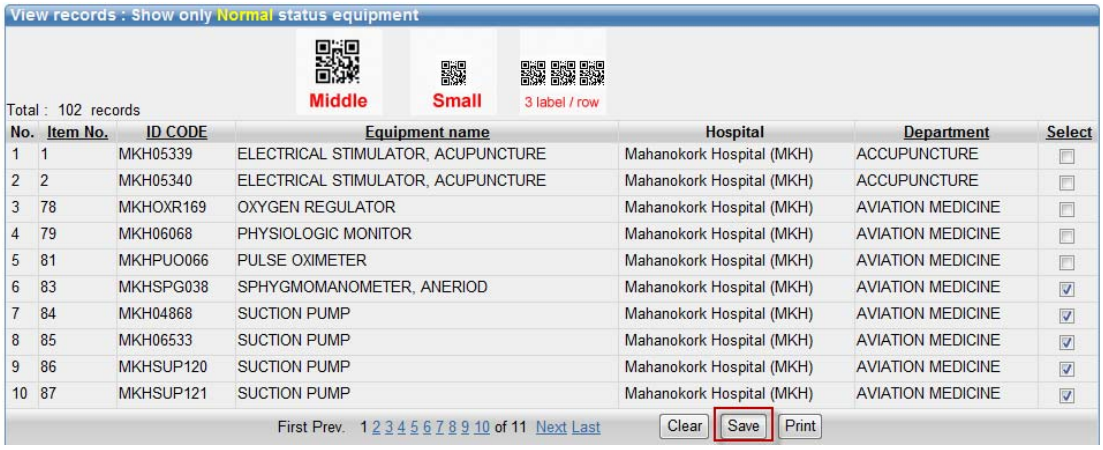
View records : Show only Normal status equipment
Middle
Small
3 label / row
Total : 102 records
No. Item No. ID CODE Equipment name Hospital Department Select
1 1 MKH05339 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
2 2 MKH05340 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
3 78 MKHOXR169 OXYGEN REGULATOR Mahanokork Hospital (MKH) AVIATION MEDICINE
4 79 MKH06068 PHYSIOLOGIC MONITOR Mahanokork Hospital (MKH) AVIATION MEDICINE
5 81 MKHPUO066 PULSE OXIMETER Mahanokork Hospital (MKH) AVIATION MEDICINE
6 83 MKHSPG038 SPHYGMOMANOMETER, ANERIOD Mahanokork Hospital (MKH) AVIATION MEDICINE
7 84 MKH04868 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
8 85 MKH06533 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
9 86 MKHSUP120 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
10 87 MKHSUP121 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
First Prev. 1 2 3 4 5 6 7 8 9 10 of 11 Next Last
Clear
Save
Print

4. Click print Label model 1 for print Middle size Label.

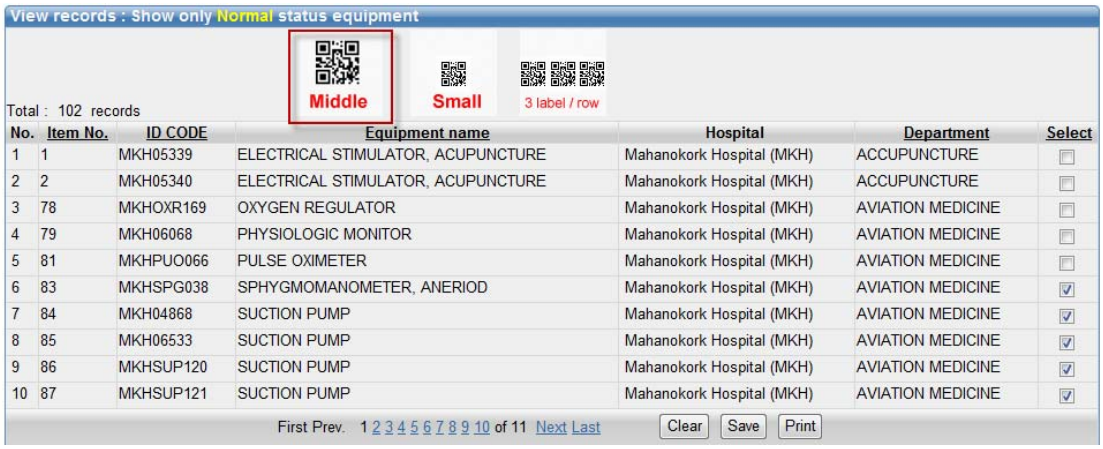
View records : Show only Normal status equipment
Middle
Small
3 label / row
Total : 102 records
No. Item No. ID CODE Equipment name Hospital Department Select
1 1 MKH05339 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
2 2 MKH05340 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
3 78 MKHOXR169 OXYGEN REGULATOR Mahanokork Hospital (MKH) AVIATION MEDICINE
4 79 MKH06068 PHYSIOLOGIC MONITOR Mahanokork Hospital (MKH) AVIATION MEDICINE
5 81 MKHPUO066 PULSE OXIMETER Mahanokork Hospital (MKH) AVIATION MEDICINE
6 83 MKHSPG038 SPHYGMOMANOMETER, ANERIOD Mahanokork Hospital (MKH) AVIATION MEDICINE
7 84 MKH04868 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
8 85 MKH06533 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
9 86 MKHSUP120 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
10 87 MKHSUP121 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
First Prev. 1 2 3 4 5 6 7 8 9 10 of 11 Next Last
Clear
Save
Print

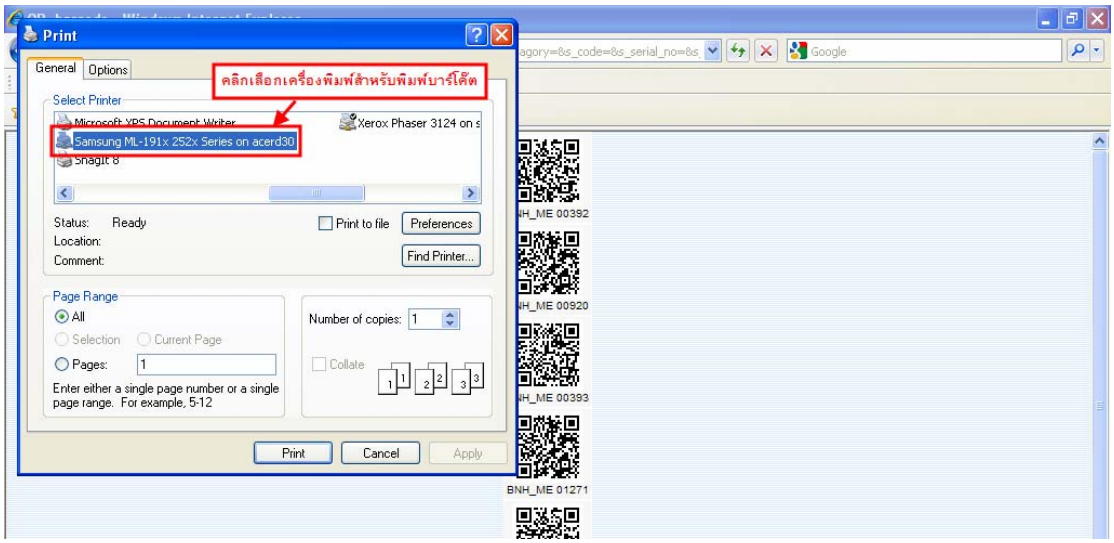

Select printer to print and click Print.

- Example of Lable (Model 1)

5. Click 2nd model print button for print small size label.

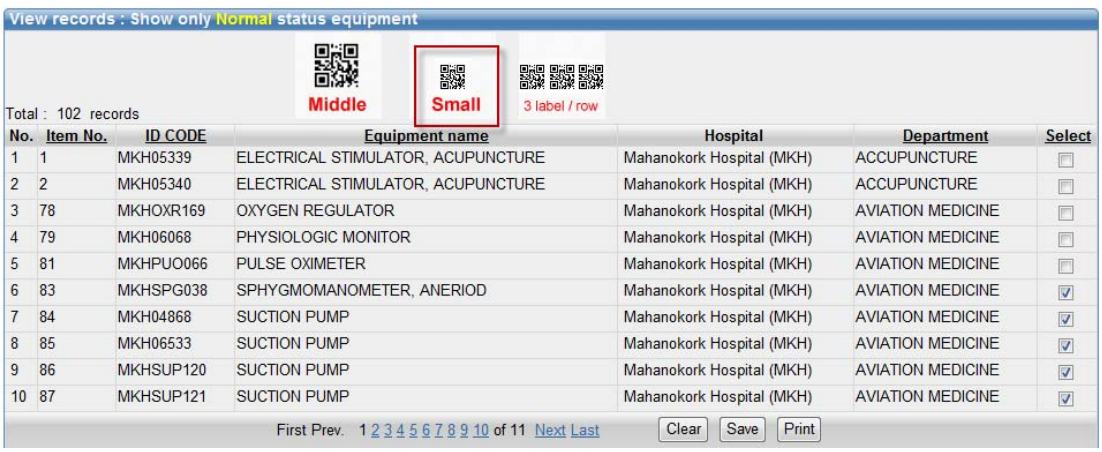
View records : Show only Normal status equipment
Middle
Small
3 label / row
Total : 102 records
No. Item No. ID CODE Equipment name Hospital Department Select
1 1 MKH05339 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
2 2 MKH05340 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
3 78 MKHOXR169 OXYGEN REGULATOR Mahanokork Hospital (MKH) AVIATION MEDICINE
4 79 MKH06068 PHYSIOLOGIC MONITOR Mahanokork Hospital (MKH) AVIATION MEDICINE
5 81 MKHPUO066 PULSE OXIMETER Mahanokork Hospital (MKH) AVIATION MEDICINE
6 83 MKHSPG038 SPHYGMOMANOMETER, ANERIOD Mahanokork Hospital (MKH) AVIATION MEDICINE
7 84 MKH04868 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
8 85 MKH06533 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
9 86 MKHSUP120 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
10 87 MKHSUP121 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
First Prev. 1 2 3 4 5 6 7 8 9 10 of 11 Next Last
Clear
Save
Print

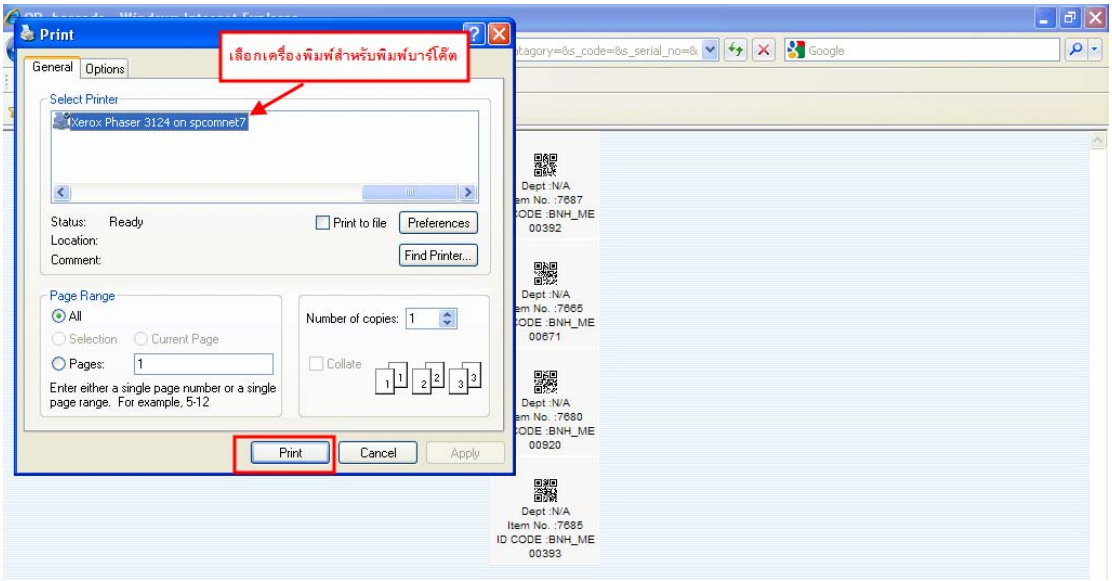

Select printer to print and click Print.

- Example of Lable (Model 2)

- Take printed Label to stick at equipment.

- Clear default setting for new selection, system will take all tick in checkbox out for new selection.

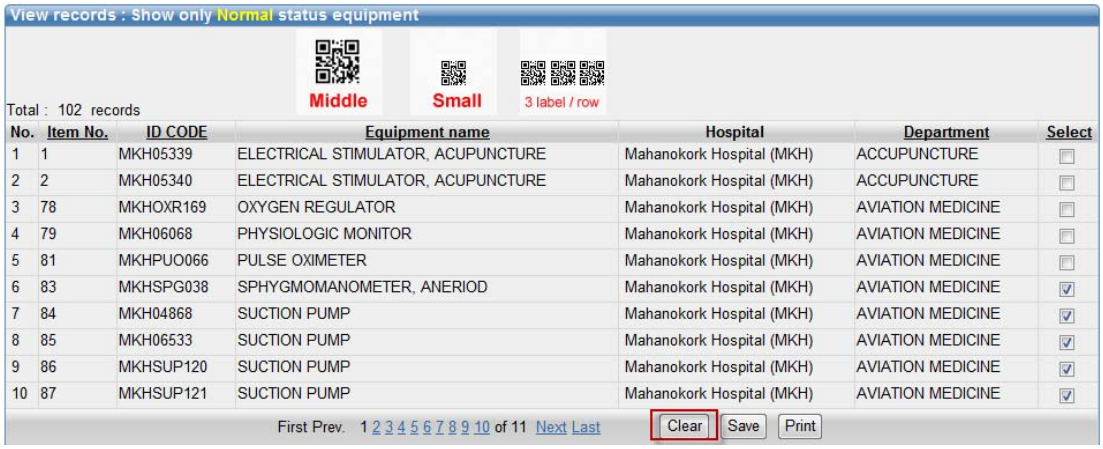
View records : Show only Normal status equipment
Middle
Small
3 label / row
Total : 102 records
No. Item No. ID CODE Equipment name Hospital Department Select
1 1 MKH05339 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
2 2 MKH05340 ELECTRICAL STIMULATOR, ACUPUNCTURE Mahanokork Hospital (MKH) ACCUPUNCTURE
3 78 MKHOXR169 OXYGEN REGULATOR Mahanokork Hospital (MKH) AVIATION MEDICINE
4 79 MKH06068 PHYSIOLOGIC MONITOR Mahanokork Hospital (MKH) AVIATION MEDICINE
5 81 MKHPUO066 PULSE OXIMETER Mahanokork Hospital (MKH) AVIATION MEDICINE
6 83 MKHSPG038 SPHYGMOMANOMETER, ANERIOD Mahanokork Hospital (MKH) AVIATION MEDICINE
7 84 MKH04868 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
8 85 MKH06533 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
9 86 MKHSUP120 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
10 87 MKHSUP121 SUCTION PUMP Mahanokork Hospital (MKH) AVIATION MEDICINE
First Prev. 1 2 3 4 5 6 7 8 9 10 of 11 Next Last
Clear
Save
Print

Print equipment register

Equipment history.

For print equipment repair history. Loggedin department can print only own department equipment repair history.

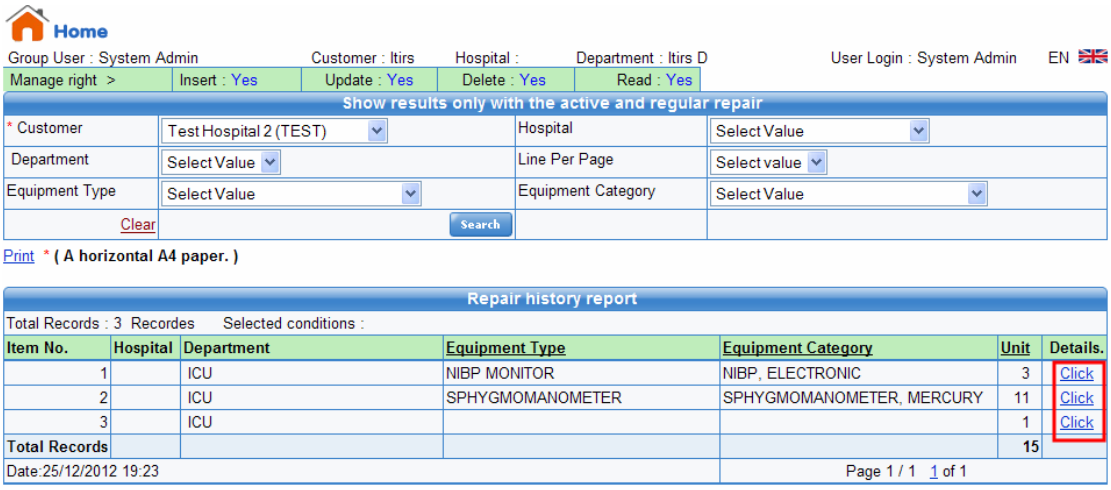
Home
Group User : System Admin
Customer : Itirs
Hospital :
Department : Itirs D
User Login : System Admin
EN
Manage right >
Insert : Yes
Update : Yes
Delete : Yes
Read : Yes
Show results only with the active and regular repair
* Customer
Test Hospital 2 (TEST)
Hospital
Select Value
Department
Select Value
Line Per Page
Select value
Equipment Type
Select Value
Equipment Category
Select Value
Clear
Search
Print * (A horizontal A4 paper.)
Repair history report
Total Records : 3 Recordes Selected conditions :
Item No. | Hospital | Department | Equipment Type | Equipment Category | Unit | Details.
1 | | ICU | NIBP MONITOR | NIBP, ELECTRONIC | 3 | Click
2 | | ICU | SPHYGMOMANOMETER | SPHYGMOMANOMETER, MERCURY | 11 | Click
3 | | ICU | | | 1 | Click
Total Records | | | | | 15 |
Date:25/12/2012 19:23
Page 1 / 1 1 of 1

➢ Click view details.

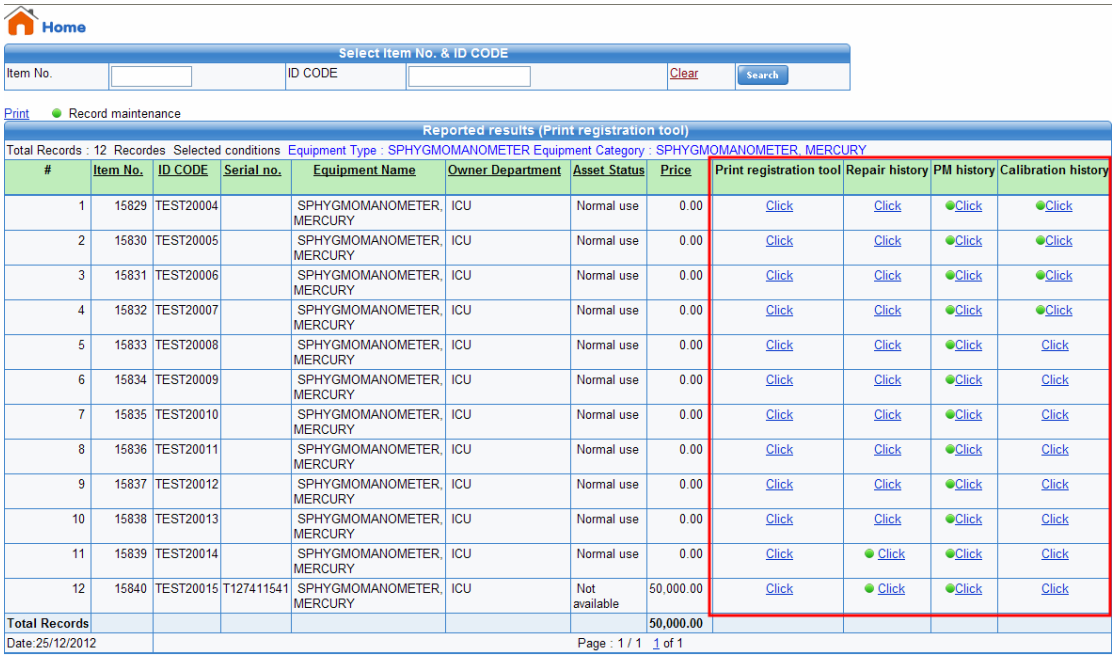
Home
Select Item No. & ID CODE
Item No.
ID CODE
Clear
Search
Print
Record maintenance
Reported results (Print registration tool)
Total Records : 12 Recordes Selected conditions Equipment Type : SPHYGMOMANOMETER Equipment Category : SPHYGMOMANOMETER, MERCURY
| Item No. | ID CODE | Serial no. | Equipment Name | Owner Department | Asset Status | Price | Print registration tool | Repair history | PM history | Calibration history
1 | 15829 | TEST20004 | | SPHYGMOMANOMETER, MERCURY | ICU | Normal use | 0.00 | Click | Click | Click | Click
2 | 15830 | TEST20005 | | SPHYGMOMANOMETER, MERCURY | ICU | Normal use | 0.00 | Click | Click | Click | Click
3 | 15831 | TEST20006 | | SPHYGMOMANOMETER, MERCURY | ICU | Normal use | 0.00 | Click | Click | Click | Click
4 | 15832 | TEST20007 | | SPHYGMOMANOMETER, MERCURY | ICU | Normal use | 0.00 | Click | Click | Click | Click
5 | 15833 | TEST20008 | | SPHYGMOMANOMETER, MERCURY | ICU | Normal use | 0.00 | Click | Click | Click | Click
6 | 15834 | TEST20009 | | SPHYGMOMANOMETER, MERCURY | ICU | Normal use | 0.00 | Click | Click | Click | Click
7 | 15835 | TEST20010 | | SPHYGMOMANOMETER, MERCURY | ICU | Normal use | 0.00 | Click | Click | Click | Click
8 | 15836 | TEST20011 | | SPHYGMOMANOMETER, MERCURY | ICU | Normal use | 0.00 | Click | Click | Click | Click
9 | 15837 | TEST20012 | | SPHYGMOMANOMETER, MERCURY | ICU | Normal use | 0.00 | Click | Click | Click | Click
10 | 15838 | TEST20013 | | SPHYGMOMANOMETER, MERCURY | ICU | Normal use | 0.00 | Click | Click | Click | Click
11 | 15839 | TEST20014 | | SPHYGMOMANOMETER, MERCURY | ICU | Normal use | 0.00 | Click | Click | Click | Click
12 | 15840 | TEST20015 | T127411541 | SPHYGMOMANOMETER, MERCURY | ICU | Not available | 50,000.00 | Click | Click | Click | Click
Total Records | | | | | | | 50,000.00
Date:25/12/2012
Page : 1 / 1 1 of 1

➢ Click print Registralation tool.

Equipment control register

Issue Date :03/01/2012 Issue No. :

Department : ICU **Department Code : 00002010001**

ID CODE : TEST20015 **Item No. :** 15840

Equipment Name :SPHYGMOMANOMETER, MERCURY
Equipment Name (English) : SPHYGMOMANOMETER, MERCURY
Brand / Model / Size :BAUMANOMETER/ 3AA/
Serial No : T127411541
Asset ID :

Equipment Type / Price	Supplier
Equipment Type :SPHYGMOMANOMETER	Supplier :CESCO LIMITED
Types of budgets :	Address Supplier :
Price (Baht) :50,000.00	Phone No. / Fax. :
How acquired :	Invoice number :
Date of receipt :03/01/2012	Producing countries :
Remark :	

Depre. Balance	Distribution
Salvage :1	Document distribution :
Date processing :11	Retire Document Date :
Accumulated depreciation current month :833.32	Retire Approve Date :
Accumulated depreciation :9,166.48	Asset Status : Not available
Accumulated depreciation current Year :9,166.48	
Book Value :40,832.52	

➢ Click print repair history.

Repair history

Item No. : 15840 ID CODE : TEST20015
Equipment : SPHYGMOMANOMETER, MERCURY Serial no. : T127411541
Customer Test Hospital 2 (TEST) Hospital Test Hospital 2
Department : ICU Autorize name : Phone no. :
Brand/Model/Size : BAUMANOMETER Receive date : 03/01/2555 Price : 50,000.00
Supplier : CESCO LIMITED

Repair history

Total : 1 times

No. of time 1 **Receive : 21/12/2012** **Symptom/Case : damage**

#Repair order 10875 **Summary :** **How to solve :**

No.	Spare parts record/Wage/Outsource	Quantity	Price/unit	Amount
1	Records not found.			
Total				

Total (Zero)

➢ Click print PM history.

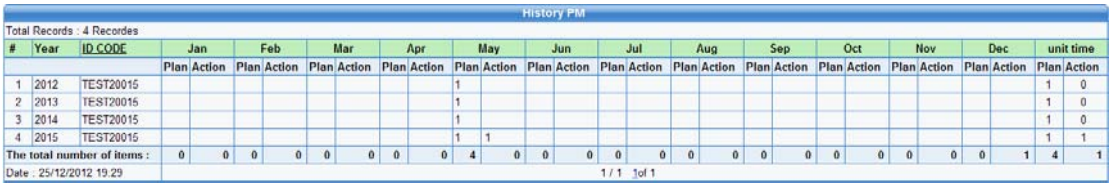

History PM

Total Records : 4 Recordes

#	Year	ID CODE	Jan		Feb		Mar		Apr		May		Jun		Jul		Aug		Sep		Oct		Nov		Dec		unit time	
			Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action
1	2012	TEST20015									1																1	0
2	2013	TEST20015									1																1	0
3	2014	TEST20015									1																1	0
4	2015	TEST20015									1	1															1	1
The total number of items :			0	0	0	0	0	0	0	0	4	0	0	0	0	0	0	0	0	0	0	0	0	0	0	1	4	1
Date : 25/12/2012 19.29			1 / 1 1of 1																									

➢ Click print Calibration history.

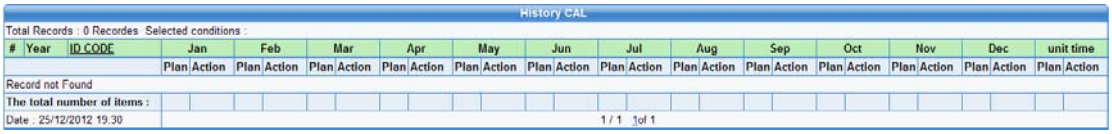

History CAL

Total Records : 0 Recordes Selected conditions :

#	Year	ID CODE	Jan		Feb		Mar		Apr		May		Jun		Jul		Aug		Sep		Oct		Nov		Dec		unit time	
			Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action	Plan	Action
Record not Found																												
The total number of items :																												
Date : 25/12/2012 19.30			1 / 1 1of 1																									